



<i>Title:</i> NEON Algorithm Theoretical Basis Document (ATBD) – Barometric Pressure		<i>Date:</i> 09/24/2024
<i>NEON Doc. #:</i> NEON.DOC.000653	<i>Author:</i> D. Smith	<i>Revision:</i> E

NEON ALGORITHM THEORETICAL BASIS DOCUMENT (ATBD) – BAROMETRIC PRESSURE

PREPARED BY	ORGANIZATION	DATE
Derek Smith	FIU	01/06/2014
Josh Roberti	FIU	02/12/2016
Jesse Vance	AQU	03/31/2016
Kaelin M. Cawley	AQU	05/30/2017
Nora Catolico	AQU	08/03/2017
Bobby Hensley	AQU	09/24/2024

APPROVALS	ORGANIZATION	APPROVAL DATE
Kate Thibault	SCI	04/20/2022

RELEASED BY	ORGANIZATION	RELEASE DATE
Tanisha Waters	CM	04/20/2022

See configuration management system for approval history.



neon
Operated by Battelle

<i>Title:</i> NEON Algorithm Theoretical Basis Document (ATBD) – Barometric Pressure		<i>Date:</i> 09/24/2024
<i>NEON Doc. #:</i> NEON.DOC.000653	<i>Author:</i> D. Smith	<i>Revision:</i> E

The National Ecological Observatory Network is a project solely funded by the National Science Foundation and managed under cooperative agreement by Battelle. Any opinions, findings, and conclusions or recommendations expressed in this material are those of the author(s) and do not necessarily reflect the views of the National Science Foundation.



Title: NEON Algorithm Theoretical Basis Document (ATBD) – Barometric Pressure		Date: 09/24/2024
NEON Doc. #: NEON.DOC.000653	Author: D. Smith	Revision: E

Change Record

REVISION	DATE	ECO #	DESCRIPTION OF CHANGE
A	08/02/2013	ECO-00796	Initial Release
B	05/04/2016	ECO-03727	Updated document to reflect L0 and L1 data product renumbering. Revised <i>Algorithm Implementation</i> and <i>Uncertainty</i> Sections. Changes include: Added <i>soil plot pressure</i> data products and input dependencies. Added HMP155 dependent L1 data products to calculate elevation corrected pressure. Aquatic meteorology station information added. Removed dynamic calculations of effective degrees of freedom and implementing a standardized coverage factor of k=2 to calculate an expanded uncertainty at 95% confidence Added footnote to CVAL reference Moved mentions of Consistency analyses to the Future Updates Section in Each ATBD Added logic table for inputs to corrected pressure equation(s)
C	12/12/2017	ECO-05282	Add buoy specific implementation of the barometric pressure sensor.
D	04/20/2022	ECO-06809	<ul style="list-style-type: none"> Update to reflect change in terminology from relocatable to gradient sites Revised logo Added Neon to document title
E	09/24/2024	ECO-07108	Updated to reflect changes to Barometric pressure above water on-buoy (DP1.20004) algorithm to no longer use water surface elevation (DP1.20016). Minor formatting changes throughout.



Title: NEON Algorithm Theoretical Basis Document (ATBD) – Barometric Pressure		Date: 09/24/2024
NEON Doc. #: NEON.DOC.000653	Author: D. Smith	Revision: E

TABLE OF CONTENTS

1 DESCRIPTION 1

 1.1 Purpose 1

 1.2 Scope..... 1

2 RELATED DOCUMENTS AND ACRONYMS 2

 2.1 Applicable Documents 2

 2.2 Reference Documents..... 2

 2.3 Acronyms 2

 2.4 Variable Nomenclature 3

 2.5 Verb Convention 3

3 DATA PRODUCT DESCRIPTION 4

 3.1 Variables Reported..... 4

 3.2 Input Dependencies 4

 3.3 Product Instances..... 8

 3.4 Temporal Resolution and Extent..... 8

 3.5 Spatial Resolution and Extent 9

4 SCIENTIFIC CONTEXT 10

 4.1 Theory of Measurement 10

 4.2 Theory of Algorithm 10

5 ALGORITHM IMPLEMENTATION..... 16

6 UNCERTAINTY..... 19

 6.1 Uncertainty of Atmospheric Pressure Measurements..... 19

 6.1.1 Measurement Uncertainty 20

 6.1.2 Uncertainty of L1 Mean Pressure Data Product 22

 6.2 Uncertainty Budget 30

7 FUTURE PLANS AND MODIFICATIONS..... 32

8 BIBLIOGRAPHY..... 33



Title: NEON Algorithm Theoretical Basis Document (ATBD) – Barometric Pressure		Date: 09/24/2024
NEON Doc. #: NEON.DOC.000653	Author: D. Smith	Revision: E

LIST OF TABLES AND FIGURES

Table 1. List of DPs used to derive L1 DPs within this ATBD (Barometric pressure NEON.DP1.00004).4

Table 2. List of DPs used to derive L1 DPs within this ATBD (Barometric Pressure on-buoy NEON.DP1.20004).7

Table 3. Logic Table for corrected pressure calculations at terrestrial sites. *Val* represents value, e.g., temperature, and whether or not $n \geq 1$ for the given averaging period. QF represents the final quality flag of said data product. *T* represents temperature, and *T_d* represents dew point.15

Table 4. Flags associated with station pressure measurements.18

Table 5. Information maintained in the CI data store for barometric pressure.18

Table 6. Uncertainty budget for individual station pressure measurements.30

Table 7. Uncertainty budget for L1 mean station and elevation corrected pressure data products. Shaded rows denote the order of uncertainty propagation (from lightest to darkest). Note that although ucTs is in terms of °C in AD[17], the uncertainty value in K is equivalent.30

Figure 1. Displays the data flow and associated uncertainties of individual pressure measurements and L1 pressure DPs. Sea level pressure is represented by *SLP*, and soil surface pressure is represented by *SSP*. For more information regarding the calibration procedure, please refer to AD [13,14,15].20



<i>Title:</i> NEON Algorithm Theoretical Basis Document (ATBD) – Barometric Pressure		<i>Date:</i> 09/24/2024
<i>NEON Doc. #:</i> NEON.DOC.000653	<i>Author:</i> D. Smith	<i>Revision:</i> E

1 DESCRIPTION

1.1 Purpose

This document details the algorithms used for creating NEON L1 DPs from L0 DPs for tower-based and on-buoy measurements of barometric pressure, and ancillary data (such as calibration data), obtained via instrumental measurements made by the Vaisala BAROCAP® Digital Barometer PTB330. It includes a detailed discussion of measurement theory and implementation, appropriate theoretical background, data product provenance, quality assurance and control methods used, approximations and/or assumptions made, and a detailed exposition of uncertainty resulting in a cumulative reported uncertainty for this product.

1.2 Scope

This document describes the theoretical background and entire algorithmic process for creating the NEON L1 data products for barometric pressure, NEON.DOM.SITE.DP1.00004.001 and barometric pressure above water on-buoy NEON.DOM.SITE.DP1.20004.001 from input data. It does not provide computational implementation details, except for cases where these stem directly from algorithmic choices explained here.



Title: NEON Algorithm Theoretical Basis Document (ATBD) – Barometric Pressure		Date: 09/24/2024
NEON Doc. #: NEON.DOC.000653	Author: D. Smith	Revision: E

2 RELATED DOCUMENTS AND ACRONYMS

2.1 Applicable Documents

AD[01]	NEON.DOC.000001	NEON OBSERVATORY DESIGN
AD[02]	NEON.DOC.005003	NEON Scientific Data Products Catalog
AD[03]	NEON.DOC.005004	NEON Level 1-3 Data Products Catalog
AD[04]	NEON.DOC.005005	NEON Level 0 Data Products Catalog
AD[05]	NEON.DOC.005505	NEON CVAL Technical and Operating Requirements
AD[06]	NEON.DOC.000735	Atmospheric Pressure Calibration Fixture
AD[07]	NEON.DOC.000782	ATBD QA/QC Data Consistency
AD[08]	NEON.DOC.011081	ATBD QA/QC plausibility tests
AD[09]	NEON.DOC.000783	ATBD De-spiking and time series analyses
AD[11]	NEON.DOC.000785	TIS Level 1 Data Products Uncertainty Budget Estimation Plan
AD[12]	NEON.DOC.000646	NEON Algorithm Theoretical Basis Document: SAATs
AD[13]	NEON.DOC.000746	Evaluating Uncertainty (CVAL)
AD[14]	NEON.DOC.000927	NEON Calibration and Sensor Uncertainty Values ¹
AD[15]	NEON.DOC.000735	CVAL Barometric Pressure Calibration Fixture
AD[16]	NEON.DOC.001113	Quality Flags and Quality Metrics for TIS Data Products
AD[17]	NEON.DOC.011083	NEON Algorithm Theoretical Basis Document – Soil CO ₂ concentration
AD[18]	NEON.DOC.001446	C ³ AQU Barometric Pressure
AD[19]	NEON.DOC.000851	NEON Algorithm Theoretical Basis Document – Relative Humidity
AD[20]	NEON.DOC.001152	Aquatic Sampling Strategy
AD[21]	NEON.DOC.003808	C ³ Buoy meteorological station and submerged sensor assembly
AD[22]	NEON.DOC.004392	Barometric pressure on-buoy ingest workbook
AD[23]	NEON.DOC.004393	Barometric pressure on-buoy publication workbook
AD[24]	NEON.DOC.002651	NEON Data Product Numbering Convention

2.2 Reference Documents

RD[01]	NEON.DOC.000008	NEON Acronym List
RD[02]	NEON.DOC.000243	NEON Glossary of Terms

2.3 Acronyms

Acronym	Explanation
AGL	Above Ground Level

¹ Note that CI obtains calibration and sensor values directly from an XML file maintained and updated by CVAL in real time. This report is updated approximately quarterly such that there may be a lag time between the XML and report updates.



Title: NEON Algorithm Theoretical Basis Document (ATBD) – Barometric Pressure		Date: 09/24/2024
NEON Doc. #: NEON.DOC.000653	Author: D. Smith	Revision: E

ASL	Above Sea Level
ATBD	Algorithm Theoretical Basis Document
CVAL	NEON Calibration, Validation, and Audit Laboratory
DAS	Data Acquisition System
DP	Data Product
FDAS	Field Data Acquisition System
L0	Level 0
L1	Level 1
LR	Lapse Rate
N/A	Not Applicable

2.4 Variable Nomenclature

The symbols used to display the various inputs in the ATBD, e.g., calibration coefficients and uncertainty estimates, were chosen so that the equations can be easily interpreted by the reader. However, the symbols provided will not always reflect NEON’s internal notation, which is relevant for CI’s use, and or the notation that is used to present variables on NEON’s data portal. Therefore a lookup table is provided below in order to distinguish what symbols specific variables can be tied to in the following document.

Symbol	Internal Notation	Description
C_0	CVALA0	CVAL calibration coefficient
C_1	CVALA1	CVAL calibration coefficient
C_2	CVALA2	CVAL calibration coefficient
u_{A1P}	UCVAL_A1	Standard combined uncertainty of station pressure; provided by CVAL.
u_{A3P}	UCVAL_A3	Calibration uncertainty of station pressure; provided by CVAL.
u_{A3T_s}	UCVAL_A3	Calibration uncertainty of station temperature; provided by CVAL.
u_{A3T_d}	UCVAL_A3	Calibration uncertainty of dewpoint; provided by CVAL.

2.5 Verb Convention

"Shall" is used whenever a specification expresses a provision that is binding. The verbs "should" and "may" express non-mandatory provisions. "Will" is used to express a declaration of purpose on the part of the design activity.



Title: NEON Algorithm Theoretical Basis Document (ATBD) – Barometric Pressure		Date: 09/24/2024
NEON Doc. #: NEON.DOC.000653	Author: D. Smith	Revision: E

3 DATA PRODUCT DESCRIPTION

3.1 Variables Reported

Pressure related L1 DPs provided by the algorithms documented in this ATBD are displayed in the accompanying file, bar_datapub_NEONDOC002884.txt (NEON.DP1.00004; tower-based measurements).

Pressure related L1 DPs for barometric pressure on-buoy (NEON.DP1.20004) can be found in the accompanying publication workbook AD[23], bar_datapub_NEONDOC004393.txt.

3.2 Input Dependencies

Table 1 and Table 2 detail the barometric pressure related L0 and L1 DPs used in this ATBD.

Table 1. List of DPs used to derive L1 DPs within this ATBD (Barometric pressure NEON.DP1.00004).

Description	Sample Frequency	Units	Data Product Number
Station Pressure	0.1 Hz	<i>kPa</i>	NEON.DOM.SITE.DP0.00004.001.01311.HOR.VER.000
One-minute mean station pressure	NA	<i>kPa</i>	NEON.DOM.SITE.DP1.00004.001.00451.HOR.VER.001
One-minute station pressure final quality flag	NA	<i>binary</i>	NEON.DOM.SITE.DP1.00004.001.00490.HOR.VER.001
One-minute station pressure expanded uncertainty	NA	<i>kPa</i>	NEON.DOM.SITE.DP1.00004.001.00456.HOR.VER.001
thirty-minute mean station pressure	NA	<i>kPa</i>	NEON.DOM.SITE.DP1.00004.001.00451.HOR.VER.030
Thirty-minute station pressure final quality flag	NA	<i>binary</i>	NEON.DOM.SITE.DP1.00004.001.00490.HOR.VER.030
Thirty-minute station pressure expanded uncertainty	NA	<i>kPa</i>	NEON.DOM.SITE.DP1.00004.001.00456.HOR.VER.030
One-minute mean temperature (soil plot HMP155)	NA	°C	NEON.DOM.SITE.DP1.00098.001.00693.HOR.000.001
One-minute temperature final quality flag (soil plot HMP155)	NA	<i>binary</i>	NEON.DOM.SITE.DP1.00098.001.00732.HOR.000.001
One-minute temperature expanded uncertainty (soil plot HMP155)	NA	°C	NEON.DOM.SITE.DP1.00098.001.00698.HOR.000.001



Title: NEON Algorithm Theoretical Basis Document (ATBD) – Barometric Pressure		Date: 09/24/2024
NEON Doc. #: NEON.DOC.000653	Author: D. Smith	Revision: E

One-minute mean temperature (tower HMP155)	NA	°C	NEON.DOM.SITE.DP1.00098.001.00693.000.VER.001
One-minute temperature final quality flag (tower HMP155)	NA	binary	NEON.DOM.SITE.DP1.00098.001.00732.000.VER.001
One-minute temperature expanded uncertainty (tower HMP155)	NA	°C	NEON.DOM.SITE.DP1.00098.001.00698.000.VER.001
Thirty-minute mean temperature (soil plot HMP155)	NA	°C	NEON.DOM.SITE.DP1.00098.001.00693.HOR.000.030
Thirty-minute temperature final quality flag (soil plot HMP155)	NA	binary	NEON.DOM.SITE.DP1.00098.001.00732.HOR.000.030
Thirty-minute temperature expanded uncertainty (soil plot HMP155)	NA	°C	NEON.DOM.SITE.DP1.00098.001.00698.HOR.000.030
Thirty-minute mean temperature (tower HMP155)	NA	°C	NEON.DOM.SITE.DP1.00098.001.00693.000.VER.030
Thirty-minute temperature final quality flag (tower HMP155)	NA	binary	NEON.DOM.SITE.DP1.00098.001.00732.000.VER.030
Thirty-minute temperature expanded uncertainty (tower HMP155)	NA	°C	NEON.DOM.SITE.DP1.00098.001.00698.000.VER.030
One-minute mean dewpoint temperature (soil plot HMP155)	NA	°C	NEON.DOM.SITE.DP1.00098.001.00733.HOR.000.001
One-minute dewpoint temperature final quality flag (soil plot HMP155)	NA	binary	NEON.DOM.SITE.DP1.00098.001.00772.HOR.000.001
One-minute dewpoint temperature expanded uncertainty (soil plot HMP155)	NA	°C	NEON.DOM.SITE.DP1.00098.001.00738.HOR.000.001
One-minute mean dewpoint temperature (tower HMP155)	NA	°C	NEON.DOM.SITE.DP1.00098.001.00733.000.VER.001
One-minute dewpoint temperature final quality flag (tower HMP155)	NA	binary	NEON.DOM.SITE.DP1.00098.001.00772.000.VER.001



Title: NEON Algorithm Theoretical Basis Document (ATBD) – Barometric Pressure		Date: 09/24/2024
NEON Doc. #: NEON.DOC.000653	Author: D. Smith	Revision: E

One-minute dewpoint temperature expanded uncertainty (tower HMP155)	NA	°C	NEON.DOM.SITE.DP1.00098.001.00738.000.VER.001
Thirty-minute mean dewpoint temperature (soil plot HMP155)	NA	°C	NEON.DOM.SITE.DP1.00098.001.00733.HOR.000.030
Thirty-minute dewpoint temperature final quality flag (soil plot HMP155)	NA	<i>binary</i>	NEON.DOM.SITE.DP1.00098.001.00772.HOR.000.030
Thirty-minute dewpoint temperature expanded uncertainty (soil plot HMP155)	NA	°C	NEON.DOM.SITE.DP1.00098.001.00738.HOR.000.030
Thirty-minute mean dewpoint temperature (tower HMP155)	NA	°C	NEON.DOM.SITE.DP1.00098.001.00733.000.VER.030
Thirty-minute dewpoint temperature final quality flag (tower HMP155)	NA	<i>binary</i>	NEON.DOM.SITE.DP1.00098.001.00772.000.VER.030
Thirty-minute dewpoint temperature expanded uncertainty (tower HMP155)	NA	°C	NEON.DOM.SITE.DP1.00098.001.00738.000.VER.030
Barometer's Latitude	NA	<i>deg. N</i>	CI data store
Barometer's elevation	NA	<i>m</i>	CI data store
uncertainty of Barometer's elevation	NA	<i>m</i>	CI data store
Center of Soil Plot 1 elevation	NA	<i>m</i>	CI data store
uncertainty of Soil Plot 1 elevation	NA	<i>m</i>	CI data store
Center of Soil Plot 2 elevation	NA	<i>m</i>	CI data store
uncertainty of Soil Plot 2 elevation	NA	<i>m</i>	CI data store
Center of Soil Plot 3 elevation	NA	<i>m</i>	CI data store
uncertainty of Soil Plot 3 elevation	NA	<i>m</i>	CI data store
Center of Soil Plot 4 elevation	NA	<i>m</i>	CI data store
uncertainty of Soil Plot 4 elevation	NA	<i>m</i>	CI data store



Title: NEON Algorithm Theoretical Basis Document (ATBD) – Barometric Pressure		Date: 09/24/2024
NEON Doc. #: NEON.DOC.000653	Author: D. Smith	Revision: E

Center of Soil Plot 5 elevation	NA	<i>m</i>	CI data store
uncertainty of Soil Plot 5 elevation	NA	<i>m</i>	CI data store

Table 2. List of DPs used to derive L1 DPs within this ATBD (Barometric Pressure on-buoy NEON.DP1.20004).

Description	Sample Frequency	Units	Data Product Number
Station Pressure	1 per minute	<i>kPa</i>	NEON.DOM.SITE.DP0.20004.001.01311.HOR.VER.000
One-minute mean station pressure	NA	<i>kPa</i>	NEON.DOM.SITE.DP1.20004.001.03421.HOR.VER.001
One-minute station pressure final quality flag	NA	<i>integer</i>	NEON.DOM.SITE.DP1.20004.001.03419.HOR.VER.001
One-minute station pressure expanded uncertainty	NA	<i>kPa</i>	NEON.DOM.SITE.DP1.20004.001.03418.HOR.VER.001
thirty-minute mean station pressure	NA	<i>kPa</i>	NEON.DOM.SITE.DP1.20004.001.03435.HOR.VER.030
Thirty-minute station pressure final quality flag	NA	<i>unsigned integer</i>	NEON.DOM.SITE.DP1.20004.001.03419.HOR.VER.030
Thirty-minute station pressure expanded uncertainty	NA	<i>kPa</i>	NEON.DOM.SITE.DP1.20004.001.03418.HOR.VER.030
One-minute mean temperature (buoy HMP155)	NA	<i>°C</i>	NEON.DOM.SITE.DP1.20271.001.00693.HOR.VER.001
One-minute temperature final quality flag (buoy HMP155)	NA	<i>integer</i>	NEON.DOM.SITE.DP1.20271.001.00732.HOR.VER.001
One-minute temperature expanded uncertainty (buoy HMP155)	NA	<i>°C</i>	NEON.DOM.SITE.DP1.20271.001.00698.HOR.VER.001
Thirty-minute mean temperature (buoy HMP155)	NA	<i>°C</i>	NEON.DOM.SITE.DP1.20271.001.00693.HOR.VER.030
Thirty-minute temperature final quality flag (buoy HMP155)	NA	<i>integer</i>	NEON.DOM.SITE.DP1.20271.001.00732.HOR.VER.030
Thirty-minute temperature expanded uncertainty (buoy HMP155)	NA	<i>°C</i>	NEON.DOM.SITE.DP1.20271.001.00698.HOR.VER.030



Title: NEON Algorithm Theoretical Basis Document (ATBD) – Barometric Pressure		Date: 09/24/2024
NEON Doc. #: NEON.DOC.000653	Author: D. Smith	Revision: E

One-minute mean dewpoint temperature (buoy HMP155)	NA	°C	NEON.DOM.SITE.DP1.20271.001.00733.HOR.V ER.001
One-minute dewpoint temperature final quality flag (buoy HMP155)	NA	<i>integer</i>	NEON.DOM.SITE.DP1.20271.001.00772.HOR.V ER.001
One-minute dewpoint temperature expanded uncertainty (buoy HMP155)	NA	°C	NEON.DOM.SITE.DP1.20271.001.00738.HOR.V ER.001
Thirty-minute mean dewpoint temperature (buoy HMP155)	NA	°C	NEON.DOM.SITE.DP1.20271.001.00733.HOR.V ER.030
Thirty-minute dewpoint temperature final quality flag (buoy HMP155)	NA	<i>integer</i>	NEON.DOM.SITE.DP1.20271.001.00772.HOR.V ER.030
Thirty-minute dewpoint temperature expanded uncertainty (buoy HMP155)	NA	°C	NEON.DOM.SITE.DP1.20271.001.00738.HOR.V ER.030
Barometer’s Latitude	NA	<i>deg. N</i>	CI data store
Barometer’s elevation	NA	<i>m</i>	CI data store
uncertainty of Barometer’s elevation	NA	<i>m</i>	CI data store

3.3 Product Instances

Barometric pressure will be recorded at all core and gradient sites through a Vaisala BAROCAP® Digital PTB330 Class A barometer.

With a slightly different configuration, an additional PTB330 Class A sensor will be deployed at all lake and river sites where the sensor will be installed on the buoy.

3.4 Temporal Resolution and Extent

Barometric pressure will be recorded at a rate of 0.1 Hz for L0, tower-based and aquatic shore based met stations, measurements. These L0 DPs will be used to calculate the one- and thirty-minute averages (L1 DPs) of station pressure, pressure corrected to sea level, and pressure corrected to soil plot heights (one-minute averages, only). Barometric pressure on buoys will be recorded at a rate of once per minute for L0 measurements. These L0 DPs will be used to calculate the one- and thirty-minute averages (L1 DPs) of station pressure and pressure corrected to sea level.



<i>Title:</i> NEON Algorithm Theoretical Basis Document (ATBD) – Barometric Pressure		<i>Date:</i> 09/24/2024
<i>NEON Doc. #:</i> NEON.DOC.000653	<i>Author:</i> D. Smith	<i>Revision:</i> E

3.5 Spatial Resolution and Extent

At terrestrial sites the pressure sensor will be located on the tower infrastructure at a site-specific installation height (h) above ground level (AGL). At aquatic sites the pressure sensor will be located on a field-based met station (tripod) at a standard installation height of above ground level. Lake and river sites will have an additional pressure sensor located on a buoy at a standard installation height above water level (AWL), but at a different sampling frequency. Therefore, barometric (station) pressure will represent the point in space at which the barometer is located.



Title: NEON Algorithm Theoretical Basis Document (ATBD) – Barometric Pressure		Date: 09/24/2024
NEON Doc. #: NEON.DOC.000653	Author: D. Smith	Revision: E

4 SCIENTIFIC CONTEXT

Barometric pressure, or static atmospheric pressure, is a vital measurement for NEON. Barometric pressure is significant in influencing weather conditions as well as aqueous chemistry (e.g. the amount of gas that can dissolve in solution). Recording static atmospheric pressure will allow atmospheric gas mixing ratios to be converted into mass quantities. Barometric pressure will be recorded over NEON’s entire operational range and the accuracy and precision requirements can be found in Dynamic Object-Oriented Requirements System.

4.1 Theory of Measurement

Simply stated, barometric pressure is the weight exerted on a given location by the atmosphere above it, per unit area. Barometric pressure has long been determined using mercury barometers, which relate the weight of the atmosphere to the weight of a column of mercury. While mercury barometers are common for many historical applications, digital, aneroid barometers are becoming much more prevalent. This is mainly attributed to their ruggedness and ability to be automated while still maintaining high accuracy and stability (Van der Meulen 1992).

Aneroid barometers operate on the principal of converting pressure proportionally to electrical voltage through the use of transducers (i.e. silicon diaphragm), microprocessors, and sensors. In the Vaisala BAROCAP® barometer, pressure is determined from changes in the capacitance of a silicon crystal sensor. CVAL’s calibration process to meet NEON’s accuracy and precision requirements can be found in AD[06].

4.2 Theory of Algorithm

Pressure will be presented as station pressure, p_s , pressure corrected to sea level, p_0 , pressure corrected to the elevation of each TIS soil plot, and pressure corrected to the elevation of each aquatic sensor set location. Station pressure will first be determined applying calibration coefficients, supplied by CVAL, to the “raw” sensor output as follows:

$$p_{s_i} = C_2 * p_i^2 + C_1 * p_i + C_0 \tag{1}$$

where:

- p_{s_i} = Individual station pressure (kPa)
- C_2 = Calibration coefficient provided by CVAL ((kPa)⁻¹)
- C_1 = Calibration coefficient provided by CVAL (unitless)
- C_0 = Calibration coefficient provided by CVAL (kPa)
- p_i = Individual pressure output from sensor (kPa)

One-minute averages of station, soil plot, and sea level pressure will be determined following Eq. (2), and thirty-minute averages of station and sea level pressure will be determined following and (3) to



Title: NEON Algorithm Theoretical Basis Document (ATBD) – Barometric Pressure		Date: 09/24/2024
NEON Doc. #: NEON.DOC.000653	Author: D. Smith	Revision: E

create the L1 DPs listed in listed in file bar_datapub_NEONDOC002884.txt and bar_datapub_NEONDOC004393.txt. Here we let p represent station, sea level, and soil plot pressure since they will be averaged the same way to create the L1 DPs according to Eq. (2) and (3). Individual calibrated measurements, i.e. 0.1 Hz pressure for tower sensors, will be made available upon request.

The on-buoy PTB330 returns data at about 1 measurement per minute. Because of the communication system at the buoys (AD[21]), it is possible that zero or more than one (probably 2 or 3 maximum) measurements will be returned per minute. Thus, for the buoy PTB330 the number of values that are averaged may not be a consistent value. Usually, 1-minute mean will be just one instantaneous measurement and 30-minute mean will be a mean of 30 measurements. When zero measurements are returned for a given minute, a timestamp and data may not be published to users.

$$\overline{p_1} = \frac{1}{n} \sum_{i=1}^n p_i \quad (2)$$

where, for each 1-minute average, n is the number of measurements during the averaging period and p_i is a pressure measurement (0.1-Hz for tower sensors and 1/60 Hz for buoy) taken during the 60-second averaging period [0, 60). For a 1-minute average, $n = 6$ for towers if all data points are included and $n = 1$ for buoys

and,

$$\overline{p_{30}} = \frac{1}{n} \sum_{i=1}^n p_i \quad (3)$$

where, for each 30-minute average, n is the number of measurements during the averaging period and p_i is a pressure measurement (0.1-Hz for tower sensors and 1/60 Hz for buoy) taken during the 1800-second averaging period [0, 1800).

Note: The beginning of the first averaging period in a series shall be the nearest whole minute less than or equal to the first timestamp in the series.

Due to the effects that temperature and altitude have on pressure, readings are often normalized to sea level so that they are analogous among locations. In addition, the pressure at the surface of each soil plot, which usually differ in elevation from the barometer, are needed to apply a compensation to the soil CO₂ concentration sensor measurements (AD[17]).

Barometric pressure at the water surface influences the rate of gas exchange between the water and atmosphere. Corrected Pressure should be derived to properly calculate the reaeration (gas exchange) rate, which is necessary to determining ecological parameters such as whole stream metabolism (Johnson, 2013). Since the on-buoy sensor is located within a few meters of the water surface the on-



buoy pressure reading is considered representative of the pressure at the water surface. This number will then be normalized to sea level based on the lake surface elevation. Within sites, the effect of variation in actual water surface elevation (NEON.DP1.20016) on barometric pressure is much smaller than other sources of uncertainty. In order to not have corrected barometric pressure be dependent on this additional data stream, lake surface elevation will be derived from the static, surveyed elevation of the lake pressure transducer, which is stored in the named location database. The geoNEON package (<https://github.com/NEONScience/NEON-geolocation>) or NEON API (<http://data.neonscience.org/api>) can be used to access the most up-to-date geospatial and location information for a particular sensor if greater pressure accuracy is needed.

The WMO (2008) presents Eq. (4), which is used to adjust station pressure to different atmospheric heights and sea level. Although other algorithms exist, the algorithm provided by the WMO (2008) is considered the standard method:

$$p_{\Lambda} = p_s * e^{\left(\frac{Z_{\phi} * \frac{g_0}{R_d}}{\bar{T}_v}\right)} = p_s * e^{\left(\frac{Z_{\phi} * \frac{g_0}{R_d}}{T_s + \frac{\alpha * Z_{\phi}}{2} + e_v * C_h}\right)} \quad (4)$$

where:

- Z_{ϕ} = Geopotential Height of barometer (gpm) Above Sea Level (ASL)
- g_0 = Standard acceleration of gravity = 9.80665 (m s⁻²)
- R_d = Gas constant of dry air = 287.05 (J kg⁻¹.K⁻¹)
- \bar{T}_v = Mean virtual temperature (K)
- α = Standard Atmospheric Lapse Rate of temperature = 0.0065 (K m⁻¹)
- p_{Λ} = $\begin{cases} p_0 & \text{when calculating sea level pressure} \\ p_{soil} & \text{when calculating soil surface pressure} \end{cases}$ (kPa)
- p_s = Station pressure (kPa)
- T_s = Station temperature (K)
- e_v = Vapor pressure (kPa)
- C_h = Lapse rate of vapor pressure = 1.2 (K kPa⁻¹; Rao 1957, 1958)

According to Wallace and Hobbs (2006), the calculation of Z_{ϕ} is:

$$Z_{\phi} \equiv \frac{\Phi(z)}{g_0} = \frac{1}{g_0} \int_c^z g(\theta, z') dz' \quad (5)$$

where:

- Z_{ϕ} = Barometer's geopotential Height (gpm) above reference level
- $\Phi(z)$ = Geopotential (m² s⁻²) at barometer's elevation
- g_0 = Globally averaged gravity (9.81 m s⁻²)
- z = Barometer's elevation (m ASL)



- $g(\theta, z')$ = Local gravity as a function of elevation and latitude of the barometer (m s^{-2})
 z' = Integration constant
 c = elevation of converted pressure reference level (m)
 $\begin{cases} 0 & \text{when calculating sea level pressure} \\ h_{soil} & \text{when calculating soil surface pressure} \end{cases}$
 $h_{soil,i}$ = elevation of the center of soil plot i (m ASL), stored in the CI data store.

The horizontal and vertical distances between the barometer on the tower and each soil plot are always <300 m, and <75 m, respectively. The difference in pressure in horizontal space is assumed to be negligible since pressure changes are considerably smaller in the horizontal relative to the vertical (Ahrens 2007). The algorithm for soil surface pressure, p_{soil} , accounts for the difference in the geopotential height (vertical distances) of the barometer and the soil plot surface.

The local gravity (m s^{-2}) at barometer height z (m), can be approximated as follows (Jursa 1985):

$$g(\theta, z) = 9.780356[1 + 0.0052885 \sin^2 \theta - 0.0000059 \sin^2(2\theta)] - 0.003086 * \left(\frac{z}{1000}\right) \quad (6)$$

where:

θ = latitude of barometer (radians), provided in the CI data store

Combining Eqns. (5) and (6):

$$Z_{\phi} * g_0 \equiv \frac{\Phi(z)}{g_0} * g_0 \equiv \Phi(z) \approx h' * g(\theta, z) \quad (7)$$

where:

$$h' = z - c \quad (8)$$

h' = Barometer's elevation (m) above reference level c

Substituting, Eq. (4) becomes:

$$p_{\Lambda} = p_s * e^{\left(\frac{Z_{\phi} * g_0}{R_d \left(\bar{T}_s + \frac{\alpha * Z}{2} + e_v * C_h\right)}\right)} \approx p_s * e^{\left(\frac{h' * g(\theta, z)}{R_d \left(\bar{T}_s + \frac{\alpha * Z}{2} + e_v * C_h\right)}\right)} \quad (9)$$

Vapor pressure, e_v , which is a function of dew point, is simply the pressure that atmospheric water vapor exerts on the atmosphere (Wallace and Hobbs 2006). Values of e_v are rarely > 3 kPa in mid-latitude regions, but can occasionally reach slightly higher values in the Subtropics and Tropics where concentrations of atmospheric water vapor are high. Vapor pressure will be derived using dewpoint data



derived from either a) the soil plot hygrometer at terrestrial sites (TIS), or b) the met station hygrometer at aquatic sites (AQU); this process is detailed in Eq. (10).

$$\bar{e}_v = 10^{\left(\frac{7.5}{\frac{237.3}{\bar{T}_d} + 1}\right) - 0.21411} \quad (10)$$

where:

\bar{e}_v : One- or thirty-minute mean vapor pressure (kPa)

$$\bar{T}_d := \begin{cases} \text{NEON. DOM. SITE. DP1.00098.001.00733. HOR. VER. 001} & (1 - \text{minute Tower}) \\ \text{OR} \\ \text{NEON. DOM. SITE. DP1.00098.001.00733. HOR. VER. 030} & (30 - \text{minute Tower}) \\ \text{OR} \\ \text{NEON. DOM. SITE. DP1.20271.001.00733. HOR. VER. 001} & (1 - \text{minute Buoy}) \\ \text{OR} \\ \text{NEON. DOM. SITE. DP1.20271.001.00733. HOR. VER. 030} & (30 - \text{minute Buoy}) \end{cases}$$

The final equation for reduction of station pressure will be:

$$\bar{p}_A = \bar{p}_s * e^{\left(\frac{h' * g(\theta, z)}{R_d \left(\bar{T}_s + \frac{\alpha * z}{2} + \bar{e}_v * c_h\right)}\right)} \quad (11)$$

where:

$$\bar{p}_A = \begin{cases} \bar{p}_0 & \text{when calculating sea level pressure (kPa)} \\ \bar{p}_{\text{soil},i} & \text{when calculating soil surface pressure (kPa), } i = \text{soil plot number} \\ \bar{p}_{\text{water},i} & \text{when calculating water surface pressure (kPa), } i = \text{sensor set number} \end{cases}$$

$$\bar{p}_s = \begin{cases} \text{NEON. DOM. SITE. DP1.00004.001.00451. HOR. VER. 001} & (1 - \text{minute Tower}) \\ \text{OR} \\ \text{NEON. DOM. SITE. DP1.00004.001.00451. HOR. VER. 030} & (30 - \text{minute Tower}) \\ \text{OR} \\ \text{NEON. DOM. SITE. DP1.20004.001.00451. HOR. VER. 001} & (1 - \text{minute Buoy}) \\ \text{OR} \\ \text{NEON. DOM. SITE. DP1.20004.001.00451. HOR. VER. 030} & (30 - \text{minute Buoy}) \end{cases}$$

$$\bar{T}_s = \begin{cases} \text{NEON. DOM. SITE. DP1.00004.001.00693. HOR. VER. 001} & (1 - \text{minute Tower}) \\ \text{OR} \\ \text{NEON. DOM. SITE. DP1.00004.001.00693. HOR. VER. 030} & (30 - \text{minute Tower}) \\ \text{OR} \\ \text{NEON. DOM. SITE. DP1.20271.001.00693. HOR. VER. 001} & (1 - \text{minute Buoy}) \\ \text{OR} \\ \text{NEON. DOM. SITE. DP1.20271.001.00693. HOR. VER. 030} & (30 - \text{minute Buoy}) \end{cases}$$



Title: NEON Algorithm Theoretical Basis Document (ATBD) – Barometric Pressure		Date: 09/24/2024
NEON Doc. #: NEON.DOC.000653	Author: D. Smith	Revision: E

L1 mean temperature (converted to Kelvin; Eq. (12)) and dew point DPs with corresponding temporal resolutions to corrected sea and surface pressures (i.e., one or thirty minute averages) shall be used as inputs to correct station pressure as shown in Eq. (10) and (11).

$$\bar{T}_s = (\bar{T}_1 \text{ or } \bar{T}_{30}) + 273.15 \tag{12}$$

Table 3 details which HMP155 sensor shall be used when deriving corrected pressure.

Table 3. Logic Table for corrected pressure calculations at terrestrial sites. *Val* represents value, e.g., temperature, and whether or not $n \geq 1$ for the given averaging period. *QF* represents the final quality flag of said data product. *T* represents temperature, and *T_d* represents dew point.

No.	Soil Plot				Tower				T QF	T _d QF	Note
	T		T _d		T		T _d				
	Val	QF	Val	QF	Val	QF	Val	QF			
1	present	0	present	0					0	0	Both ground present and both QF=0
2					present	0	present	0	0	0	Both tower present and both QF=0
3	present	0/1	present	0/1					0/1	0/1	Both ground present but either QF=1
4					present	0/1	present	0/1	0/1	0/1	Both tower present but either QF=1
5	Do not compute										

At buoy sites the one-minute mean temperature from the HMP155 sensor will be used as station temperature (\bar{T}_s) and the one-minute mean dew point from the HMP155 sensor will be used for dew point temperature (T_d).



Title: NEON Algorithm Theoretical Basis Document (ATBD) – Barometric Pressure		Date: 09/24/2024
NEON Doc. #: NEON.DOC.000653	Author: D. Smith	Revision: E

5 ALGORITHM IMPLEMENTATION

Data flow for signal processing of L1 DPs will be treated in the following order.

1. The barometer L0 DPs will be converted into station pressure by applying calibration coefficients through Eq. (1).
2. QA/QC Plausibility tests will be applied to the data stream in accordance with AD[08]. The details are provided below.
3. Signal de-spiking will be applied to the data stream in accordance with AD[09].
4. One- and thirty-minute station barometric pressure averages will be calculated using Eq. (2) and (3).
5. Descriptive statistics, i.e. minimum, maximum, and variance, will be determined for both one- and thirty-minute averages of station pressure.
6. Quality metrics, quality flags, and the final quality flag will be produced for one- and thirty-minute station pressure averages according to AD[16].
7. One- and thirty-minute averages of station pressure will be converted to corrected sea and surface pressures through Eq. (11).
8. QA/QC sensor flags will be applied to the data stream for corrected sea and surface pressures, details provided below.
9. The final quality flag for corrected sea and surface pressures will be produced as detailed below.

QA/QC Procedure:

1. **Plausibility Tests** AD[08] – All plausibility tests will be determined for the barometer. Test parameters will be provided by FIU and maintained in the CI data store. All plausibility tests will be applied to the sensor’s converted L0 DPs and associated quality flags (QFs) will be generated for each test.
2. **Sensor Flags** – Barometric pressure corrected to sea level (i.e., corPres) and surface level (i.e., surfacePres) require ambient temperature and dew point measurements as inputs. In the event this ancillary data is unavailable or flagged the following quality flags shall be set accordingly.

a. Temperature:

tempQF=	1 if temperature sensor measurements are missing or flagged (details in Section 4.2)
	0 otherwise

b. Dew Point:

	1 if dew point sensor measurements are missing or flagged (details in Section 4.2)
--	--



Title: NEON Algorithm Theoretical Basis Document (ATBD) – Barometric Pressure		Date: 09/24/2024
NEON Doc. #: NEON.DOC.000653	Author: D. Smith	Revision: E

$$\text{dewPointQF} = \begin{cases} 1 & \text{if } \text{tempQF} = 1 \text{ or } \text{dewPointQF} = 1 \\ 0 & \text{otherwise} \end{cases}$$

3. **Signal De-spiking** – Time segments and threshold values for the automated despiking QA/QC routine will be specified by FIU and maintained in the CI data store. QFs from the despiking analysis will be applied according to AD[09].
4. **Quality Flags (QFs) and Quality Metrics (QMs)** AD[16] – If a datum fails one of the following tests it will not be used to create a L1 DP, *range*, *persistence*, and *step*. α and β QFs and QMs will be determined for station pressure using the flags in **Table 4**. In addition, station pressure L1 DPs will have a QA/QC report and quality metrics associated with each flag listed in **Table 4**, as detailed in AD[16]. Ancillary information needed for the algorithm and other information maintained in the CI data store is shown in **Table 5**. Since corrected sea and surface pressures are determined by converting the mean station pressure their quality information only includes temperature, dew point, and final quality flags. The final quality flag for station pressure, pressure corrected to sea level, and pressure corrected to surface level will be determined accordingly.

a. Final Quality

- i. **Station Pressure** – The final quality flag for station pressure (i.e., staPresFinalQF) shall be set as well as detailed in AD[16].
- ii. **Pressure Corrected to Sea Level** – The final quality flag for pressure corrected to sea level shall be set to one if the final flag for station pressure was 1 or, determined accordingly as shown below.

$$\text{corPresFinalQF} = \begin{cases} 1 & \text{if } \text{staPresFinalQF} = 1 \text{ or } \text{tempQF} = 1 \text{ or } \text{dewPointQF} = 1 \\ 0 & \text{otherwise} \end{cases}$$

- iii. **Pressure Corrected to Surface Level** – The final quality flag for pressure converted to surface level shall be set to one if the final flag for station pressure was 1 or, determined accordingly as shown below.

$$\text{surfacePresFinalQF} = \begin{cases} 1 & \text{if } \text{staPresFinalQF} = 1 \text{ or } \text{tempQF} = 1 \text{ or } \text{dewPointQF} = 1 \\ 0 & \text{otherwise} \end{cases}$$



Title: NEON Algorithm Theoretical Basis Document (ATBD) – Barometric Pressure		Date: 09/24/2024
NEON Doc. #: NEON.DOC.000653	Author: D. Smith	Revision: E

Table 4. Flags associated with station pressure measurements.

Tests
Range
Persistence
Step
Null
Gap
Valid Calibration
Signal Despiking
Alpha
Beta
Final quality flag

Table 5. Information maintained in the CI data store for barometric pressure.

Tests/Values	CI Data Store Contents
Range	Minimum and maximum values
Persistence	Window size, threshold values and maximum time length
Step	Threshold values
Null	Test limit
Gap	Test limit
Valid Calibration	CVAL sensor specific valid calibration date range
Signal Despiking	Time segments and threshold values
Calibration	CVAL sensor specific calibration coefficients
Uncertainty	AD[14]
Final Quality Flag	AD[16]

6 UNCERTAINTY

Uncertainty of measurement is inevitable; therefore, measurements should be accompanied by a statement of their uncertainty for completeness (JCGM 2008; Taylor 1997). To do so, it is imperative to identify all sources of measurement uncertainty related to the quantity being measured. Quantifying the uncertainty of TIS measurements will provide a measure of the reliability and applicability of individual measurements and TIS data products. This portion of the document serves to identify, evaluate, and quantify sources of uncertainty relating to individual, calibrated pressure measurements as well as L1 mean pressure DPs. It is a reflection of the information described in AD[11], and is explicitly described for the barometric assembly in the following sections.

6.1 Uncertainty of Atmospheric Pressure Measurements

Uncertainty of the pressure assembly is discussed in this section. This section discusses two topics. The first informs the sources of *measurement* uncertainty, i.e., those associated with *individual measurements*. The second details uncertainties associated with temporally averaged data products. A diagram detailing the data flow and known sources of uncertainty are displayed in

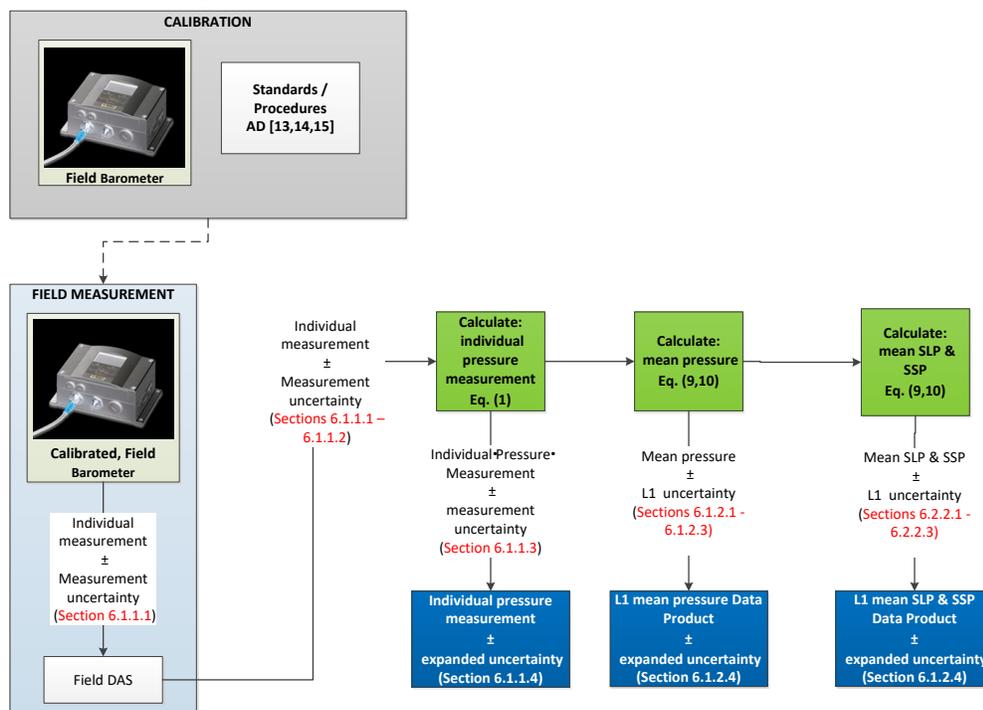


Figure 1.

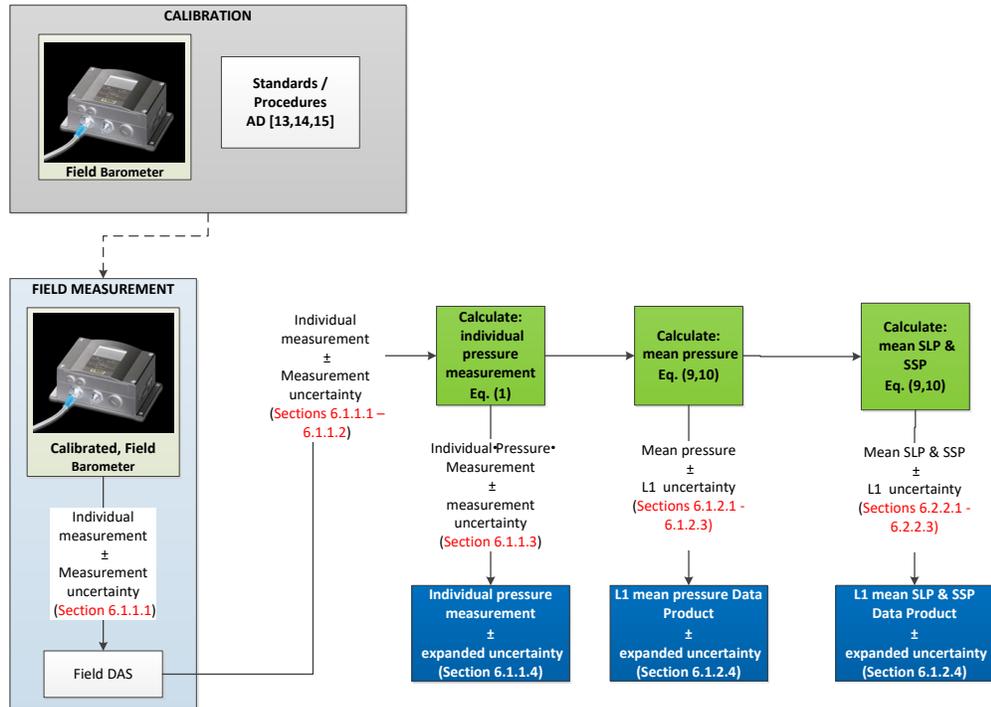


Figure 1. Displays the data flow and associated uncertainties of individual pressure measurements and L1 pressure DPs. Sea level pressure is represented by *SLP*, and soil surface pressure is represented by *SSP*. For more information regarding the calibration procedure, please refer to AD [13,14,15].

6.1.1 Measurement Uncertainty

The following subsections present the uncertainties associated with *individual pressure observations*. It is important to note that the uncertainties presented in the following subsections are *measurement uncertainties*, that is, they reflect the uncertainty of an *individual* measurement. These uncertainties should not be confused with those presented in **Section 6.1.2**. We urge the reader to refer to AD[11] for further details concerning the discrepancies between quantification of measurement uncertainties and L1 uncertainties.

NEON calculates measurement uncertainties according to recommendations of the Joint Committee for Guides in Metrology (JCGM) 2008. In essence, if a measurand y is a function of n input quantities x_i ($i = 1, \dots, n$), *i.e.*, $y = f(x_1, x_2, \dots, x_n)$, the combined measurement uncertainty of y , assuming the inputs are independent, can be calculated as follows:

$$u_c(y) = \left(\sum_{i=1}^N \left(\frac{\partial f}{\partial x_i} \right)^2 u^2(x_i) \right)^{\frac{1}{2}} \quad (13)$$

where:

- $\frac{\partial f}{\partial x_i}$ = partial derivative of y with respect to x_i
- $u(x_i)$ = combined standard uncertainty of x_i .



Title: NEON Algorithm Theoretical Basis Document (ATBD) – Barometric Pressure		Date: 09/24/2024
NEON Doc. #: NEON.DOC.000653	Author: D. Smith	Revision: E

Thus, the uncertainty of the measurand can be found by summing the input uncertainties in quadrature. For temperature measurements, the sources of uncertainty are depicted in Figure 1. The calculation of these input uncertainties is discussed below.

6.1.1.1 Station Pressure

This section details measurement uncertainties relating to individual *station* pressure measurements.

6.1.1.1.1 Calibration

Uncertainties associated with the barometer’s calibration process propagate into a standard, combined measurement uncertainty. This combined uncertainty, u_{A1p} , represents i) the repeatability and reproducibility of the sensor and the lab DAS and ii) uncertainty of the calibration procedures and coefficients including uncertainty in the standard (truth). It is a constant value that will be provided by CVAL (AD[14]), stored in the CI data store, and applied to all *individual measurements* (that is, it does not vary with any specific sensor, DAS component, location, etc.). A detailed summary of the calibration procedures and corresponding uncertainty estimates can be found in AD[13,14,15].

6.1.1.1.2 Field DAS

This barometer has an internal A/D converter and outputs data in digital form. Because of this, uncertainty introduced by the field DAS is considered negligible.

6.1.1.1.3 Dynamic Pressure (wind-induced uncertainties)

When measuring atmospheric pressure, the goal is to quantify the *static* pressure, s , of the atmosphere. The static pressure can be thought of as atmospheric pressure free from the effects of wind loading or wind-induced pressure changes (error); this phenomenon is often referred to as *dynamic pressure*, d . Atmospheric pressure can be represented by *total* pressure, t , because the effects of dynamic pressure cannot be accurately quantified.

$$s = t - d \tag{14}$$

Dynamic pressure produces a pressure error:

$$u_d(s) = \frac{\rho u^2}{2} \tag{15}$$

where:

$u(s)$ = uncertainty of static pressure introduced by dynamic pressure (kPa); equation modified from Brock and Richardson (2001)

ρ = density of the air (kg m^{-3})

u = wind velocity (m s^{-1})



Title: NEON Algorithm Theoretical Basis Document (ATBD) – Barometric Pressure		Date: 09/24/2024
NEON Doc. #: NEON.DOC.000653	Author: D. Smith	Revision: E

According to Vaisala (2012) high wind speeds can induce noticeable pressure instability when quantifying atmospheric pressure via the PTB300. The extent to which dynamic pressure affects NEON’s atmospheric pressure measure measurements is currently beyond the scope of this document. As NEON’s vector component wind data are analyzed, the magnitudes of dynamic pressure influences may be better understood.

6.1.1.1.4 Combined Measurement Uncertainty

Because CVAL’s uncertainty is the sole uncertainty associated with station pressure, the combined uncertainty for an individual measurement is simply equal to u_{A1p} .

6.1.1.1.5 Expanded Measurement Uncertainty

The expanded measurement uncertainty is calculated as:

$$U_{95}(p_{s_i}) = k_{95} * u_{A1} \tag{16}$$

where:

- $U_{95}(p_{s_i})$ = expanded measurement uncertainty at 95% confidence (kPa)
- k_{95} = 2 (unitless); coverage factor for 95% confidence

6.1.2 Uncertainty of L1 Mean Pressure Data Product

The following subsections discuss uncertainties associated with L1 mean data products. As stated previously, it is important to note the differences between the *measurement uncertainties* presented in **Section 6.1.1**, **Section 6.1.2**, and the uncertainties presented in the following subsections. The uncertainties presented in the following subsections reflect the variance of a mean value, that is, they reflect the uncertainty of a distribution of temperature measurements collected under non-controlled conditions (i.e., those found in the field), as well as any uncertainty, in the form of trueness, introduced by the field DAS and those associated with the calibration process.

6.1.2.1 Station Pressure

6.1.2.1.1 Repeatability (natural variation)

To quantify the uncertainty in the L1 mean station pressure attributable to random effects, the distribution of the individual measurements is used. Specifically, the *standard error of the mean (natural variation)*, is computed. This value, given in units of kPa, reflects the repeatability of station pressure measurements for a specified time period:



Title: NEON Algorithm Theoretical Basis Document (ATBD) – Barometric Pressure		Date: 09/24/2024
NEON Doc. #: NEON.DOC.000653	Author: D. Smith	Revision: E

$$u_{NAT}(\bar{p}_s) = \frac{s(p_s)}{\sqrt{n}} \tag{17}$$

Where $s(p_s)$ is the experimental standard deviation of individual station pressure observations for the specified averaging period and n represents the number of observations used to calculate \bar{p}_s .

6.1.2.1.2 Calibration

The uncertainty detailed here is similar to that described in **Section 6.1.1.1**. However, the uncertainty of the mean DP, u_{A3} , does not consider i) individual sensor repeatability, or ii) the variation of sensors' responses over a population (reproducibility). This component estimates the calibration uncertainty, a quantity which is not captured by the standard error of the mean. It is a constant value that will be provided by CVAL (AD [14]) and stored in the CI data store. Please refer to AD[11] for further justification regarding evaluation and quantification of this combined uncertainty.

6.1.2.1.3 Combined uncertainty (mean Station Pressure)

The combined uncertainty for our L1 mean station pressure data product, $u_c(\bar{p}_s)$, given in units of kPa, is computed by summing the uncertainties from **Sections 6.1.2.1.1 and 6.1.2.1.2** in quadrature:

$$u_c(\bar{p}_s) = \left(u_{NAT}^2(\bar{p}_s) + u_{A3p}^2 \right)^{\frac{1}{2}} \tag{18}$$

6.1.2.1.4 Expanded uncertainty (mean Station Pressure)

The expanded uncertainty is calculated as:

$$U_{95}(\bar{p}_s) = k_{95} * u_c(\bar{p}_s) \tag{19}$$

where:

- $U_{95}(\bar{p}_s)$ = expanded L1 mean, station pressure, data product uncertainty at 95% confidence (kPa)
- k_{95} = 2 (unitless); coverage factor for 95% confidence

6.1.2.2 Elevation Corrected Pressure

This section details elevation corrected pressure data products. Level 1, mean, station pressure DPs will be corrected to sea level via Eq. (11), a slightly altered version of WMO's (2008) standard method. This equation comprises a great deal of uncertainty because it abides by the concept of the "standard atmosphere." Additionally, atmospheric constants (i.e., R_d and α) are subject to their own uncertainties (Henrion and Fischhoff 1986).



Title: NEON Algorithm Theoretical Basis Document (ATBD) – Barometric Pressure		Date: 09/24/2024
NEON Doc. #: NEON.DOC.000653	Author: D. Smith	Revision: E

6.1.2.2.1 Station Pressure

The partial derivative of Eq. (11) with respect to \bar{p}_s must be calculated in order to identify the sensitivity coefficient of station pressure:

$$\frac{\partial \bar{p}_\Lambda}{\partial \bar{p}_s} = e^{\left(\frac{h' * g(\theta, z)}{R_d \left(\bar{T}_s + \frac{\alpha * z}{2} + \bar{e}_v * C_h \right)} \right)} \quad (20)$$

To derive the partial uncertainty of elevation corrected pressure as a function of station pressure, the absolute value of this sensitivity coefficient is multiplied by the combined uncertainty of station pressure u_{A1} :

$$u_{\bar{p}_s}(\bar{p}_\Lambda) = \left| \frac{\partial \bar{p}_\Lambda}{\partial \bar{p}_s} \right| * u_c(\bar{p}_s) \quad [kPa] \quad (21)$$

Where, $u_c(\bar{p}_s)$ is the combined uncertainty of the L1, mean, station pressure DP and is defined by:

$$u_c(\bar{p}_s) = U_{95}(\bar{p}_s) / k_{95} \quad [kPa] \quad (22)$$

$$U_{95}(\bar{p}_s) = \begin{cases} \text{NEON. DOM. SITE. DP1.00004.001.00456. HOR. VER. 001} & (1 - \text{minute Tower}) \\ \text{OR} \\ \text{NEON. DOM. SITE. DP1.00004.001.00456. HOR. VER. 030} & (30 - \text{minute Tower}) \\ \text{OR} \\ \text{NEON. DOM. SITE. DP1.20004.001.00456. HOR. VER. 001} & (1 - \text{minute Buoy}) \\ \text{OR} \\ \text{NEON. DOM. SITE. DP1.20004.001.00456. HOR. VER. 030} & (30 - \text{minute Buoy}) \end{cases}$$

6.1.2.2.2 Elevation of Barometer and Corrected Pressure Reference Level

The barometer's and soil plot's elevations Above Sea Level (ASL) are also sources of uncertainty that propagate into the combined uncertainty of elevation corrected pressure. These uncertainties will be provided by SYS ENG and maintained in the CI data store.

The sensitivity coefficient with respect to the barometer's elevation ASL is approximately:

$$\frac{\partial \bar{p}_\Lambda}{\partial z} \approx \frac{4 * g(\theta, z) * \bar{p}_s * (\bar{T}_s + \bar{e}_v * C_h) * e^{\left(\frac{h' * g(\theta, z)}{R_d \left(\bar{T}_s + \frac{\alpha * z}{2} + \bar{e}_v * C_h \right)} \right)}}{(\alpha * z + 2(\bar{T}_s + \bar{e}_v * C_h))^2 * R_d} \quad (23)$$



Where the approximation arises from the assumption that $\frac{\partial}{\partial z}(z * g(\theta, z)) \approx g(\theta, z)$.

The partial uncertainty of pressure corrected to the reference level is:

$$u_z(\bar{p}_\Lambda) = \left| \frac{\partial \bar{p}_\Lambda}{\partial z} \right| * u(h') \quad [kPa] \quad (24)$$

where:

$$u(h') = (u^2(z) + u^2(c))^{\frac{1}{2}} \quad [kPa] \quad (25)$$

6.1.2.2.3 Acceleration of Gravity

As displayed in Eq. (6), local gravity is a function of station elevation ASL and latitude. Given the current technology of GPS, and noting that even relatively large (~1000 m) changes in elevation in the lower atmosphere result in minute changes in local gravity (~0.1 m s⁻²), we argue that the uncertainty of local gravity is negligible.

6.1.2.2.4 Dry Air Constant

A minor pitfall associated with using the dry air constant within any equation is that it assumes the atmosphere is free of water vapor. It can be said that the use of the dry air constant could cause asymmetric (systematic) uncertainty within an equation because it always assumes a completely dry atmosphere. However, in the case of correcting station pressure to a different elevation, this systematic uncertainty is corrected through the use of virtual temperature, which accounts for atmospheric moisture. In theory, the pressure of a region can be expressed as:

$$p = \rho R_d T_v = \rho R_m T \quad (26)$$

where ρ is the density of the air, R_m is the moist air constant, and T is temperature.

The dry air constant, R_d , is the gas constant for 1 kg of dry air. It is a function of the *universal gas constant* R^* (8.3145 J K⁻¹ mol⁻¹) and the apparent molecular weight of dry air M_d (28.97 g)

$$R_d = 1000 \frac{8.3145}{28.97} = 287.05 \text{ J K}^{-1} \text{ kg}^{-1} \quad (27)$$

Since it is a constant, it is considered to be a true value. We know from JCGM (2008) that a true value can never be measured, and universal constants will always comprise a level of uncertainty (Henrion and Fischhoff 1986). However, the magnitude of this uncertainty is most likely minimal, especially when



compared to those of the other variables comprising Eq. (11). Thus, we can assume that the uncertainty of pressure due to the dry air constant is negligible.

6.1.2.2.5 Station Temperature

The uncertainty of the L1 mean temperature DP will be calculated via the algorithms discussed in AD[12]. This uncertainty should represent the same temporal averaging period as the resulting L1 pressure DP. For example, when calculating the *one-minute* L1 mean station pressure DP, the corresponding *one-minute* L1 mean temperature DP should be used.

The sensitivity coefficient of Eq. (11) with respect to \bar{T}_s is:

$$\frac{\partial \bar{p}_\Lambda}{\partial \bar{T}_s} = \frac{-4g(\theta, z) * \bar{p}_s * z * e^{\left(\frac{h' * g(\theta, z)}{R_d(\bar{T}_s + \frac{\alpha * z}{2} + \bar{e}_v * C_h)}\right)}}{(\alpha * z + 2(\bar{T}_s + \bar{e}_v * C_h))^2 * R_d} \quad (28)$$

The partial uncertainty of elevation corrected pressure as a function of station temperature is then:

$$u_{\bar{T}_s}(\bar{p}_\Lambda) = \left| \frac{\partial \bar{p}_\Lambda}{\partial \bar{T}_s} \right| * u_c(\bar{T}_s) \quad [kPa] \quad (29)$$

Where, $u_c(\bar{T}_s)$ is the combined uncertainty of the L1, mean temperature data product from the HMP155 used to correct station pressure and is defined by:

$$u_c(\bar{T}_s) = u_{95}(\bar{T}_s) / k_{95} \quad [kPa] \quad (30)$$

If using data from the soil plot HMP155:

$$U_{95}(\bar{T}_s) = \begin{cases} \text{NEON. DOM. SITE. DP1.00098.001.00698. HOR. 000.001} & (1 - \text{minute}) \\ \text{OR} \\ \text{NEON. DOM. SITE. DP1.00098.001.00698. HOR. 000.030} & (30 - \text{minute}) \end{cases}$$

If using data from the tower HMP155:

$$U_{95}(\bar{T}_s) = \begin{cases} \text{NEON. DOM. SITE. DP1.00098.001.00698.000. VER. 001} & (1 - \text{minute}) \\ \text{OR} \\ \text{NEON. DOM. SITE. DP1.00098.001.00698.000. VER. 030} & (30 - \text{minute}) \end{cases}$$

If using data from the buoy HMP155:

$$U_{95}(\bar{T}_s) = \begin{cases} \text{NEON. DOM. SITE. DP1.20271.001.00698. HOR. VER. 001} & (1 - \text{minute}) \\ \text{OR} \\ \text{NEON. DOM. SITE. DP1.20271.001.00698. HOR. VER. 030} & (30 - \text{minute}) \end{cases}$$



6.1.2.2.6 Lapse Rate of Temperature

As mentioned before, the standard atmospheric lapse rate is 0.0065 K m^{-1} (WMO 2008). Although this can be considered as “constant”, it holds a great deal of uncertainty because it is somewhat fictitious in nature. Atmospheric lapse rates (LR) can vary between 0.005 K m^{-1} (moist adiabatic lapse rate) and 0.01 K m^{-1} (dry adiabatic lapse rate), and can occasionally reach extremes on either side (Wallace and Hobbs 2006). To account for these variations we take a fairly liberal approach and assume this lapse rate is reliable to 80% and derive a relative uncertainty estimate of 20%:

$$u(\alpha) = \alpha * 0.20 = 0.0065 * 0.20 = 0.0013 \quad (31)$$

The partial derivative of Eq. (11) with respect to α is:

$$\frac{\partial \bar{p}_\Lambda}{\partial \alpha} = \frac{-2g(\theta, z) * \bar{p}_s * z^2 * e^{\left(\frac{h' * g(\theta, z)}{R_d(\bar{T}_s + \frac{\alpha * z}{2} + \bar{e}_v * C_h)}\right)}}{(\alpha * z + 2(\bar{T}_s + \bar{e}_v * C_h))^2 * R_d} \quad (32)$$

The partial uncertainty of elevation corrected pressure as a function of temperature’s lapse rate is then:

$$u_\alpha(\bar{p}_\Lambda) = \left| \frac{\partial \bar{p}_\Lambda}{\partial \alpha} \right| u(\alpha) \quad [kPa] \quad (33)$$

6.1.2.2.7 Vapor Pressure

Because vapor pressure is back calculated from dewpoint measurements made throughout NEON’s Observatory (see Eq. (10)), the combined uncertainty of the one-minute, mean dewpoint data product (soil plot or AQU met station) will propagate through to vapor pressure.

The derivative of corrected pressure with respect to vapor pressure can be partitioned as follows:

$$\frac{\partial \bar{p}_\Lambda}{\partial \bar{T}_d} = \frac{\partial \bar{p}_\Lambda}{\partial \bar{e}_v} * \frac{d\bar{e}_v}{d\bar{T}_d} \quad (34)$$

where:

$$\frac{\partial \bar{p}_\Lambda}{\partial \bar{T}_d} = \text{derivative of Eq. (11) with respect to } \bar{T}_d$$

$$\frac{\partial \bar{p}_\Lambda}{\partial \bar{e}_v} = \text{partial derivative of Eq. (11) with respect to } \bar{e}_v$$

$$\frac{d\bar{e}_v}{d\bar{T}_d} = \text{derivative of Eq. (10) with respect to } \bar{T}_d$$



Title: NEON Algorithm Theoretical Basis Document (ATBD) – Barometric Pressure		Date: 09/24/2024
NEON Doc. #: NEON.DOC.000653	Author: D. Smith	Revision: E

Total and partial derivatives are derived below.

$$\frac{\partial \bar{p}_\Lambda}{\partial \bar{e}_v} = \frac{-4\bar{p}_s * g(\theta, z) * C_h * z * e^{\left(\frac{h' * g(\theta, z)}{R_d(\bar{T}_s + \frac{\alpha * z}{2} + \bar{e}_v * C_h)}\right)}}{(\alpha * z + 2(\bar{T}_s + \bar{e}_v * C_h))^2 * R_d} \quad (35)$$

To show how this uncertainty affects that of vapor pressure, the partial derivative of Eq. (10) with respect to dewpoint must be derived:

$$\frac{\partial \bar{e}_v}{\partial \bar{T}_d} = \frac{1779.75 * \ln(10) * 10^{\left(\frac{7.5}{\frac{237.3}{\bar{T}_d} + 1}\right) - 0.21411}}{\left(\frac{237.3}{\bar{T}_d} + 1\right)^2 * \bar{T}_d^{-2}} \quad (36)$$

The partial uncertainty of an individual corrected pressure measurement with respect to ambient dewpoint is thus:

$$u_{\bar{T}_d}(\bar{p}_\Lambda) = \left| \frac{\partial \bar{p}_\Lambda}{\partial \bar{T}_d} \right| u_c(\bar{T}_d) \quad [kPa] \quad (37)$$

Where, $u_c(\bar{T}_d)$ is the combined uncertainty of the L1, mean dew point temperature data product from the HMP155 used to correct station pressure and is defined by:

$$u_c(\bar{T}_d) = u_{95}(\bar{T}_d) / k_{95} \quad [^\circ C] \quad (38)$$

If using data from the soil plot HMP155:

$$U_{95}(\bar{T}_d) = \begin{cases} \text{NEON. DOM. SITE. DP1.00098.001.00738. HOR. 000.001} & (1 - \text{minute}) \\ \text{OR} \\ \text{NEON. DOM. SITE. DP1.00098.001.00738. HOR. 000.030} & (30 - \text{minute}) \end{cases}$$

If using data from the tower HMP155:

$$U_{95}(\bar{T}_d) = \begin{cases} \text{NEON. DOM. SITE. DP1.00098.001.00738. HOR. VER. 001} & (1 - \text{minute}) \\ \text{OR} \\ \text{NEON. DOM. SITE. DP1.00098.001.00738. HOR. VER. 030} & (30 - \text{minute}) \end{cases}$$

If using data from the buoy HMP155:



Title: NEON Algorithm Theoretical Basis Document (ATBD) – Barometric Pressure		Date: 09/24/2024
NEON Doc. #: NEON.DOC.000653	Author: D. Smith	Revision: E

$$U_{95}(\bar{T}_d) = \begin{cases} \text{NEON.DOM.SITE.DP1.20271.001.00738.HOR.VER.001} & (1 - \text{minute}) \\ \text{OR} \\ \text{NEON.DOM.SITE.DP1.20271.001.00738.HOR.VER.030} & (30 - \text{minute}) \end{cases}$$

Overall, the impact of vapor pressure is quite small when compared to other variables in the elevation corrected pressure equation (WMO 1964).

6.1.2.2.8 Lapse Rate of Vapor Pressure

The lapse rate of vapor pressure is adapted by the WMO (1964) and incorporated into the sea level reduction equation. It is based on seasonal variation of vapor pressure within the lower atmosphere (Rao 1958). Like that of temperature, the lapse rate of vapor pressure is considered to hold a great deal of uncertainty. This is especially true over large elevation ranges. Here we take a similar, liberal approach to that of quantifying the uncertainty of temperature lapse rate and use a relative uncertainty of 20%:

$$u(C_h) = C_h * 0.20 = 1.2 * 0.20 = 0.24 \quad (39)$$

Its associated sensitivity coefficient is:

$$\frac{\partial \bar{p}_\Lambda}{\partial C_h} = \frac{-4\bar{p}_s * g(\theta, z) * \bar{e}_v * z * e^{\left(\frac{h' * g(\theta, z)}{R_d(\bar{T}_s + \frac{\alpha * z}{2} + \bar{e}_v * C_h)}\right)}}{(\alpha * z + 2(\bar{T}_s + \bar{e}_v * C_h))^2 * R_d} \quad (40)$$

And its propagating term is:

$$u_{C_h}(\bar{p}_\Lambda) = \left| \frac{\partial \bar{p}_\Lambda}{\partial C_h} \right| u(C_h) \quad [kPa] \quad (41)$$

6.1.2.2.9 Combined Uncertainty (mean Corrected Pressure)

The combined uncertainty for our L1 mean elevation corrected pressure data product, $u_c(\bar{p}_\Lambda)$, given in units of kPa, is computed by summing the uncertainties from **Sections 6.1.2.2.1** and **6.1.2.2.8** in quadrature:

$$u_c(\bar{p}_\Lambda) = \left(u_{\bar{p}_s}^2(\bar{p}_\Lambda) + u_z^2(\bar{p}_\Lambda) + u_{\bar{T}_s}^2(\bar{p}_\Lambda) + u_\alpha^2(\bar{p}_\Lambda) + u_{\bar{T}_d}^2(\bar{p}_\Lambda) + u_{C_h}^2(\bar{p}_\Lambda) \right)^{\frac{1}{2}} \quad (42)$$

6.1.2.2.10 Expanded Uncertainty (mean Corrected Pressure)

The expanded uncertainty is then calculated as:



Title: NEON Algorithm Theoretical Basis Document (ATBD) – Barometric Pressure		Date: 09/24/2024
NEON Doc. #: NEON.DOC.000653	Author: D. Smith	Revision: E

$$U_{95}(\bar{p}_A) = k_{95} * u_c(\bar{p}_A) \tag{43}$$

where:

$$U_{95}(\bar{p}_A) = \text{expanded uncertainty at 95\% confidence (kPa)}$$

$$k_{95} = 2 \text{ (unitless); coverage factor for 95\% confidence}$$

6.1.2.3 Communicated Precision

Calibrations by NEON’s CVAL reveal that the repeatability of barometer is significant to a hundred-thousandth of a kPa (or a hundredth of a Pa). As such, the communicated precision of L1, mean, barometric pressure data will be 0.00001 kPa.

6.2 Uncertainty Budget

Uncertainty budgets (**Table 6**, **Table 7**) are visual aids detailing i) quantifiable sources of uncertainty, ii) means by which they are derived, and iii) the order of their propagation. Uncertainty values denoted in this budget are either derived within this document or are provided by other NEON teams (e.g., CVAL), and stored in the CI data store.

Table 6. Uncertainty budget for individual station pressure measurements.

Source of measurement uncertainty	Measurement uncertainty component $u(x_i)$	Value of measurement uncertainty	$\frac{\partial f}{\partial x_i}$	$u_{x_i}(Y) \equiv \left \frac{\partial f}{\partial x_i} \right u(x_i)$ [kPa]
Station pressure	u_{A1}	u_{A1} [kPa]	n/a	n/a

Table 7. Uncertainty budget for L1 mean station and elevation corrected pressure data products. Shaded rows denote the order of uncertainty propagation (from lightest to darkest). Note that although $u_c(T_s)$ is in terms of °C in AD[17], the uncertainty value in K is equivalent.

Source of uncertainty	Uncertainty component $u(x_i)$	Value of uncertainty	$\frac{\partial f}{\partial x_i}$	$u_{x_i}(Y) \equiv \left \frac{\partial f}{\partial x_i} \right u(x_i)$ [kPa]
Station pressure	$u_c(\bar{p}_s)$	Eq. (18) [kPa]	n/a	n/a
Natural variation	$u_{NAT}(\bar{p}_s)$	Eq. (17) [kPa]	1	Eq. (17)
Station Pressure ^{CAL}	u_{A3_p}	u_{A3_p} [kPa]	1	u_{A3}
Corrected pressure	$u_c(p_{A_i})$	Eq. (42) [kPa]	n/a	n/a
Station pressure	u_{A1}	u_{A1} [kPa]	Eq. (20)	Eq. (21)
Elevation ¹	$u(h')$	Eq. (25) [m]	Eq. (23)	Eq. (24)



Title: NEON Algorithm Theoretical Basis Document (ATBD) – Barometric Pressure		Date: 09/24/2024
NEON Doc. #: NEON.DOC.000653	Author: D. Smith	Revision: E

Temperature	$u_c(\bar{T}_s)$	AD[12] [K]	Eq. (28)	Eq. (29)
Temperature LR	$u(\alpha)$	0.0013 [K km ⁻¹]	Eq. (32)	Eq. (33)
Vapor pressure ²	$u_c(\bar{T}_d)$	AD[19] [°C]	Eq. (34)	Eq. (37)
Vapor pressure LR	$u(C_h)$	0.24 [K kPa ⁻¹]	Eq. (40)	Eq. (41)
Corrected pressure	$u_c(p_{\Delta_i})$	Eq. (42) [kPa]	n/a	n/a

¹soil plot / water surface pressure

²propagation of dewpoint

^{CAL}Calibration uncertainty



<i>Title:</i> NEON Algorithm Theoretical Basis Document (ATBD) – Barometric Pressure		<i>Date:</i> 09/24/2024
<i>NEON Doc. #:</i> NEON.DOC.000653	<i>Author:</i> D. Smith	<i>Revision:</i> E

7 FUTURE PLANS AND MODIFICATIONS

Details concerning the evaluation and quantification of Sensor drift will be added to the uncertainty section.

QA/QC tests may be expanded to include consistency analyses among similar measurement streams.

Ideally, future updates to the buoy Campbell CR1000 data logger will allow for barometric data to stream at the same frequency as the tower sensors of 0.1 Hz.



Title: NEON Algorithm Theoretical Basis Document (ATBD) – Barometric Pressure		Date: 09/24/2024
NEON Doc. #: NEON.DOC.000653	Author: D. Smith	Revision: E

8 BIBLIOGRAPHY

- Ahrens, C. D. (2007) *Meteorology Today: An introduction to Weather, Climate, and the Environment*. Thomson Brooks/Cole. pp. 537.
- Brock, F. V., and S. J. Richardson (2001) *Meteorological Measurement Systems*. Oxford University Press. pp. 290.
- Bureau International des Poids et Mesures (BIPM) (1901) General conference on weights and measures, 70.
- Henion, M., and B. Fischhoff (1986), Assessing uncertainty in physical constants, *Am. J. Phys.*, 54, 791-798, doi :10.1119/1.14447.
- Johnson, H. 2013. Reaeration Measurements by Diffusion Dome. EPA-SESDPROC-505-R3. U.S. Environmental Protection Agency, Science and Ecosystem Support Division, Athens GA.
- Joint Committee for Guides in Metrology (JCGM) (2008) *Evaluation of measurement data – Guide to the expression of uncertainty in measurement*. pp. 120.
- JCGM (2012) *International vocabulary of metrology – Basic and general concepts and associated terms (VIM)*. 3rd Edition. pp. 92
- Jursa, A. S., (1985) *Handbook of Geophysics and the Space Environment*, 4th ed., Air Force Geophysics Laboratory, pp. 14-17.
- Met One Instruments, Inc. (1997) *Fan Aspirated Radiation Shield: Specification Sheet*. Rev. 076B, pp. 2. (K:\FIU\TIS Assemblies\3. Aspirated Air Temp-single\Manuals)
- Rao, K.N. (1957) *Regression of Vapour Pressure with Height, Latitude and Longitude*. Bombay.
- Rao, K.N. (1958) *Contribution of the humidity term in the formula for reduction of pressure to sea level*. Bombay.
- Taylor, J. R. (1997) *An Introduction to Error Analysis: The Study of Uncertainties in Physical Measurements*. University Science Books, Mill Valley, California. 2nd Ed. pp. 327.
- Vaisala (2008) *Vaisala BAROCAP digital barometer PTB330*. Vaisala Oyj, pp. 139.
- Vaisala (2009) *Vaisala PTB330 Digital Barometer for Professional Meteorology, Aviation, and Industrial Users: Technical Information*. Ref. B210708EN-B. pp.2 (P:\FIU\TIS Assemblies\9. Barometric Pressure\Manuals)
- Vaisala (2012) *Vaisala BAROCAP Digital Barometer PTB330: User's Guide*. Vaisala Oyj, pp. 144.
- Van der Meulen, J.P. (1992) *The WMO automatic digital barometer intercomparison*. WMO, WMO Technical Document 474, pp. 106.
- Wallace, J. M., and P. V. Hobbs (2006) *Atmospheric Science: An Introduction Survey*. Academic Press. 2nd Ed. pp. 483.



<i>Title:</i> NEON Algorithm Theoretical Basis Document (ATBD) – Barometric Pressure		<i>Date:</i> 09/24/2024
<i>NEON Doc. #:</i> NEON.DOC.000653	<i>Author:</i> D. Smith	<i>Revision:</i> E

World Meteorological Organization (WMO) (1964) Note on the Standardization of Pressure Reduction Methods in the International Network of Synoptic Stations. WMO Technical Note No. 61, WMO-No. 154.TP.74, Geneva.

WMO (2008) Measurement of Atmospheric Pressure. Guide to Meteorological Instruments and Methods of Observation. 8th Ed. pp. 1.3-1 – 1.3-25.