

| | | |
|--|-------------------------|-----------------------|
| <i>Title:</i> TOS Protocol and Procedure: Litterfall and Fine Woody Debris | <i>Author:</i> K. Jones | <i>Date:</i> 9/9/2014 |
| <i>NEON Doc. #:</i> NEON.DOC.001710 | | <i>Revision:</i> A |


TOS PROTOCOL AND PROCEDURE: LITTERFALL AND FINE WOODY DEBRIS

| PREPARED BY: | ORGANIZATION: | DATE: |
|---------------------|----------------------|--------------|
| Katie Jones | FSU | 9/8/2014 |
| Courtney Meier | FSU | 9/8/2014 |

| APPROVALS (Name): | ORGANIZATION: | APPROVAL DATE: |
|--------------------------|----------------------|-----------------------|
| Dave Tazik | SCI | 9/8/2014 |
| Mike Stewart | PSE | 9/8/2014 |
| | | |
| | | |

| RELEASED BY (Name): | ORGANIZATION: | RELEASE DATE: |
|----------------------------|----------------------|----------------------|
| Stephen Craft | PSE | 9/8/2014 |

See Configuration Management System for Approval History



| | | |
|--|-------------------------|-----------------------|
| <i>Title:</i> TOS Protocol and Procedure: Litterfall and Fine Woody Debris | <i>Author:</i> K. Jones | <i>Date:</i> 9/9/2014 |
| <i>NEON Doc. #:</i> NEON.DOC.001710 | | <i>Revision:</i> A |

Change Record

| REVISION | DATE | ECO # | DESCRIPTION OF CHANGE |
|-----------------|-------------|--------------|------------------------------|
| A | 9/9/2014 | ECO-02136 | Initial release |
| | | | |
| | | | |

| | | |
|---|------------------|----------------|
| Title: TOS Protocol and Procedure: Litterfall and Fine Woody Debris | Author: K. Jones | Date: 9/9/2014 |
| NEON Doc. #: NEON.DOC.001710 | | Revision: A |

TABLE OF CONTENTS

1 Description 1

 1.1 Purpose 1

 1.2 Scope 1

 1.3 Acknowledgements 1

2 Related Documents and Acronyms 2

 2.1 Applicable Documents 2

 2.2 Reference Documents 2

 2.3 Acronyms 2

 2.4 Definitions 3

3 Background and Objectives 4

 3.1 Background 4

 3.2 NEON Science Requirements 5

 3.3 NEON Data Products 5

4 Protocol 6

 4.1 Sampling methods 6

 4.2 Spatial distribution of sampling 7

5 Quality Assurance and Control 9

6 Safety 11

7 Personnel Requirements 12

8 Training Requirements 13

9 Sample Frequency and Timing 14

 9.1 Sampling Frequency and Timing 14

 9.2 Criteria for Determining Sampling Dates 14

 9.3 Sampling Frequency 15

 9.4 Sampling Timing Parameters 15

10 Standard Operating Procedures 16

 SOP A: Preparing for Sampling 16

 1. Field Equipment and Materials 16

 2. Gather necessary resources for field work 17

 SOP B: Field Sampling – Trap Deployment 18

| | | |
|---|------------------|----------------|
| Title: TOS Protocol and Procedure: Litterfall and Fine Woody Debris | Author: K. Jones | Date: 9/9/2014 |
| NEON Doc. #: NEON.DOC.001710 | | Revision: A |

- 1. Field Equipment and Materials 18
- 2. Selecting litter trap location strategy 19
- 3. Locating targeted elevated trap location..... 19
- 4. Locating random elevated trap location..... 20
- 5. Locating ground trap clip strip 23
- 5. Elevated trap construction and installation..... 23
- SOP C: Field Sampling 25
 - 1. Field Equipment and Materials 25
 - 2. Fine litter collection – Elevated traps 26
 - 3. Woody litter collection - Ground 27
- SOP D: Laboratory Processing and Analyses..... 28
 - 1. Laboratory Equipment and Materials..... 28
 - 2. Laboratory processing..... 29
 - 3. Grinding dried litter for archive and chemical analysis 31
- SOP E: Data Entry and Verification 32
 - 1. Entering and Uploading Field Data 32
 - 2. Equipment Maintenance, Cleaning and Storage 33
- 11 References 34
- Appendix A Quick references 35
- Appendix B Checklists..... 36
- Appendix C Site Specific Considerations 37
- Appendix D Site specific sampling dates 38
- Appendix E Using and Calibrating the TruPulse 360R Laser Rangefinder..... 42

LIST OF TABLES AND FIGURES

- Table 1. Size limits for functional groups collected in Elevated and Ground litter traps; litter material larger than described here will be collected according to the coarse woody debris protocol RD[10]. 6
- Table 2. Sample timing and frequency by vegetation type. 15
- Table 3. Field Equipment List for SOP A. 16
- Table 4. Field Equipment List for trap deployment 18
- Table 5. Equipment list for Field Sampling of elevated and ground litter traps..... 25
- Table 6. Prescribed “trapCondition” codes..... 26
- Table 7. Modified trapCondition codes for ground traps. 27

| | | |
|---|------------------|----------------|
| Title: TOS Protocol and Procedure: Litterfall and Fine Woody Debris | Author: K. Jones | Date: 9/9/2014 |
| NEON Doc. #: NEON.DOC.001710 | | Revision: A |

Table 8. Laboratory Equipment List for SOP D..... 28

Table 9. Elevated trap litter functional group codes 29

Table 10. Ground trap litter functional group codes 29

Table 11. Laser Target Modes available for the TruPulse 360 laser rangefinder/clinometer models. 47

Figure 1. Example of numbering system for qualifying patches of vegetation within a plot 20

Figure 2. A 20 m x 20 m NEON plot) showing the locations of 0.5m x 3m clip-harvest “cells” (dashed blue lines). Larger plots will have different nested subplots, but the coordinate numbering system for the 20 m subplot within these plots will follow the same conventions as shown above..... 21

Figure 3. Fully constructed elevated litter trap, NEON traps will have legs attached on corners rather than center (photo from Muller-Landau and Wright 2010)..... 24

Figure 4. Example field collection label. 26

Figure 5. The tilt-sensor calibration routine for the TruPulse 360R laser rangefinder. The blue arrow and line indicate the direction of the lens at each calibration step. 43

Figure 6. The internal compass calibration routine for the TruPulse 360R laser rangefinder..... 46

| | | |
|------------------------------|------------------|----------------------|
| Title: | Author: K. Jones | Date: [Publish Date] |
| NEON Doc. #: NEON.DOC.001710 | | Revision: * |

1 DESCRIPTION

1.1 Purpose

The primary purpose of this document is to provide a change-controlled version of Observatory protocols and procedures. This document provides the content for training and field-based materials for NEON staff and contractors. Documentation of content changes (i.e. changes in particular tasks or safety practices) will occur via this change-controlled document, not through field manuals or training materials.

This document is a detailed description of the field data collection, relevant pre- and post-field tasks, and safety issues as they relate to this procedure and protocol.

1.2 Scope

This document relates the tasks for a specific field sampling or laboratory processing activity and directly associated activities and safety practices. This document does not describe:

- general safety practices
- site-specific safety practices
- general equipment maintenance

It does identify procedure-specific safety hazards and associated safety requirements such as safe handling of small mammals or safe use of required chemicals and reagents.

1.3 Acknowledgements

This protocol is modeled closely after the litter monitoring protocol written by Helene C. Muller-Landau and S. Joseph Wright (2010) for the CTFS Global Forest Carbon Research Initiative.

| | | |
|------------------------------|-------------------------|-----------------------------|
| <i>Title:</i> | <i>Author:</i> K. Jones | <i>Date:</i> [Publish Date] |
| NEON Doc. #: NEON.DOC.001710 | | <i>Revision:</i> * |

2 RELATED DOCUMENTS AND ACRONYMS

2.1 Applicable Documents

Applicable documents contain information that shall be applied in the current document. Examples are higher level requirements documents, standards, rules and regulations.

| | | |
|---------|-----------------|---|
| AD [01] | NEON.DOC.004300 | EHS Safety Policy and Program Manual |
| AD [02] | NEON.DOC.004316 | Operations Field Safety and Security Plan |
| AD [03] | NEON.DOC.000724 | Domain Chemical Hygiene Plan and Biosafety Manual |
| AD [04] | NEON.DOC.000xxx | NEON Training Plan |
| AD [05] | NEON.DOC.050005 | Field Operations Job Instruction Training Plan |

2.2 Reference Documents

Reference documents contain information complementing, explaining, detailing, or otherwise supporting the information included in the current document.

| | | |
|---------|-----------------|---|
| RD [01] | NEON.DOC.000008 | NEON Acronym List |
| RD [02] | NEON.DOC.000243 | NEON Glossary of Terms |
| RD [03] | NEON.DOC.000914 | NEON Science Design for Plant Biomass, Productivity, and Leaf Area Index |
| RD [04] | NEON.DOC.005003 | NEON Scientific Data Products Catalog |
| RD [05] | NEON.DOC.014051 | Field Audit Plan |
| RD [06] | NEON.DOC.000824 | Data and Data Product Quality Assurance and Control Plan |
| RD [07] | NEON.DOC.001271 | Protocol for Manual Data Entry |
| RD [08] | NEON.DOC.014037 | TOS Protocol and Procedure: Measurement of Herbaceous Biomass |
| RD [09] | NEON.DOC.001025 | TOS Protocol and Procedure: Plot Establishment |
| RD [10] | NEON.DOC.001711 | TOS Field and Lab Protocol for Coarse Woody Debris |
| RD [11] | NEON.DOC.001924 | NEON Raw Data Ingest Workbook for TOS Litterfall and Fine Woody Debris |
| RD [12] | NEON.DOC.002132 | Datasheets for TOS Protocol and Procedure: Litterfall and Fine Woody Debris |

2.3 Acronyms

| | |
|------|--------------------------------------|
| ANPP | Aboveground Net Primary Productivity |
| SOP | Standard Operating Procedure |
| | |
| | |

| | | |
|-------------------------------------|-------------------------|-----------------------------|
| <i>Title:</i> | <i>Author:</i> K. Jones | <i>Date:</i> [Publish Date] |
| <i>NEON Doc. #:</i> NEON.DOC.001710 | | <i>Revision:</i> * |

2.4 Definitions

A **protocol** is a formal summary description of a procedure and its related rationale, and includes information on knowledge and resources needed to implement the procedure. A procedure is a set of prescribed actions that must take place to achieve a certain result, and can also be called a method. It differs from a science design in that science designs provide a more complete description of the rationale for selecting specific protocols. It differs from a training manual in that training manuals provide materials in support of skills acquisition in the topic areas including information on how to best train staff rather than detailing only the steps of the procedure.

Litterfall is defined as shed leaves and needles, reproductive parts (i.e. flowers, fruits, cones, seeds, etc.), and fine woody debris with butt-end diameter < 2 cm (modified from Clark et al. 2001, Bernier et al. 2008). Woody pieces with diameter \geq 2 cm are considered coarse woody debris, and will be sampled according to the NEON Field and Lab Protocol for Coarse Woody Debris (RD[10]).

| | | |
|------------------------------|------------------|----------------------|
| Title: | Author: K. Jones | Date: [Publish Date] |
| NEON Doc. #: NEON.DOC.001710 | | Revision: * |

3 BACKGROUND AND OBJECTIVES

3.1 Background

Quantifying production of litterfall and fine woody debris is required to estimate annual Aboveground Net Primary Productivity (ANPP) at plot, site and continental scales, and will provide essential data for understanding vegetative C fluxes over time. Litterfall and fine woody debris production will be estimated within Tower plots on an annual basis. Sampling point selection within a plot or subplot will be random, sampling points will be selected from the same randomized list generated to guide clip strip locations for herbaceous clip harvest. In ecosystems where the overstory is non-continuous (i.e. patchy) litterfall and fine woody debris sampling will be targeted rather than random across the plot.

This design calls for sorting fresh litter into specified functional groups prior to drying if time permits. If it is logistically not feasible to sort fresh material before drying, litter may be sorted after drying as time allows. However, sorting freshly collected litter is preferable because dry litter is easily fragmented and identifying small litter fragments to functional group will introduce uncertainty in sorting accuracy.

Elevated litter trap size has been selected to be consistent with existing standards and are the same dimensions (70 cm x 70 cm x 80 cm) as traps used by CTFS. To minimize the number of clip strips dedicated to fine woody debris sampling, which are therefore unavailable for herbaceous biomass sampling, ground traps will have the same dimensions as a single clip strip cell, 3 m x 0.5 m. If it is apparent that the volume of litterfall biomass collected from elevated and ground litter traps is too great to efficiently dry and process given limitations on drying oven space in the NEON laboratory, trap size or number may be reduced by Science Operations based on sample optimization analysis.

This protocol is divided into five Standard Operating Procedures (SOPs), each SOP addresses one discrete task and may be utilized as a standalone document as needed for specific field or lab tasks.

- **SOP A: Preparation for field work.** Includes gathering the necessary equipment and preloading the GPS with the necessary waypoints.
- **SOP B: Installation of Elevated and Ground Litter Traps.** Describes the steps for locating sampling points and establishing litter trap pairs.
- **SOP C: Litterfall and Fine Woody Debris Sampling.** Describes field collection of litterfall and fine woody debris from traps.
- **SOP D: Processing Litter Samples in the Laboratory.** Covers laboratory processing including drying and weighing of samples.
- **SOP E: Data Entry.** Provides guidance for manual data transcription from paper data sheets to the Access database.

| | | |
|-------------------------------------|-------------------------|-----------------------------|
| <i>Title:</i> | <i>Author:</i> K. Jones | <i>Date:</i> [Publish Date] |
| <i>NEON Doc. #:</i> NEON.DOC.001710 | | <i>Revision:</i> * |

3.2 NEON Science Requirements

This protocol fulfills Observatory science requirements that reside in NEON’s Dynamic Object-Oriented Requirements System (DOORS). Copies of approved science requirements have been exported from DOORS and are available in NEON’s document repository, or upon request.

3.3 NEON Data Products

Execution of this protocol procures samples and/or generates raw data satisfying NEON Observatory scientific requirements. These data and samples are used to create NEON data products, and are documented in the NEON Scientific Data Products Catalog (RD[04]).

| | | |
|------------------------------|------------------|----------------------|
| Title: | Author: K. Jones | Date: [Publish Date] |
| NEON Doc. #: NEON.DOC.001710 | | Revision: * |

4 PROTOCOL

To measure litterfall and fine woody debris, NEON will employ two types of sampling units: 1) square, elevated, mesh litter traps; and 2) rectangular, ground “traps” (Figure 2 SOP B). Elevated litter traps are designed to be large enough that the average size of abundant foliage and fine woody debris elements are easily intercepted by the trap. Ground traps are intended to intercept particularly large foliage elements that will not fit in elevated traps (e.g. palm fronds), and fine woody debris pieces that are too long to be sampled in elevated traps including small diameter branches.

4.1 Sampling methods

For both elevated and ground traps, only the portion of material that meets both the length and diameter criteria will be sampled (Muller-Landau and Wright 2010). Litter sampled from elevated traps will be sorted into functional groups following collection, using the groupings outlined in Table 1. Note these functional groups differ from those used in NEON’s herbaceous clip harvest protocol (RD[08]).

Table 1. Size limits for functional groups collected in Elevated and Ground litter traps; litter material larger than described here will be collected according to the coarse woody debris protocol RD[10].

| Functional Group | Elevated Traps | Ground Traps |
|---|---------------------------------------|---------------------------------------|
| Leaves | < 50 cm length | > 50 cm length |
| Needles | < 50 cm length | > 50 cm length |
| Twigs/branches | < 2 cm diameter AND < 50 cm length | < 2 cm diameter AND > 50 cm length |
| Woody material (e.g. cones, bark, etc) | < 2 cm diameter AND < 50 cm length | < 2 cm diameter AND > 50 cm length |
| Seeds | All | N/A |
| Flowers | All | N/A |
| Other (lichen, mosses, unidentifiable material, etc.) | All | N/A |

To ensure the accuracy of annual litter production estimates, ground traps will be cleared of all relevant litter material following the annual sampling bout.

Sorted litter from both elevated and ground traps will be shipped to external laboratories to be analyzed for C, N, $\delta^{13}\text{C}$ and, $\delta^{15}\text{N}$.

| | | |
|------------------------------|------------------|----------------------|
| Title: | Author: K. Jones | Date: [Publish Date] |
| NEON Doc. #: NEON.DOC.001710 | | Revision: * |

Laboratory processing

Following collection and sorting in the field, litter will be transported back to the laboratory and dried at 65°C until water weight has been removed, to within the allowed variance indicated in SOP D (minimum 48 hrs). The woody portion of litter will be cut to fit in the drying oven then dried at a higher temperature than litterfall, 105 °C to release bound water (Williamson and Wiemann 2010).

Equipment

Design of PVC elevated litter traps is adopted from the Smithsonian Tropical Research Institute Centre for Tropical Forest Studies (STRI/CTFS). Non-oxidizable metal rods (e.g. aluminum, galvanized steel, or equivalent) will be used to hold elevated litter traps in place. The corners of ground traps will be marked with non-oxidizable metal or plastic stakes to facilitate precise re-measurement of the selected sampling area.

4.2 Spatial distribution of sampling

Consistent with existing protocols, NEON will establish one elevated litter trap and one paired ground trap per 400 m² plot/subplot in Tower plots.

Only plots with woody vegetation present will be selected for litter sampling using this protocol. Vegetation surveys conducted during site characterization will inform plot selection. Initially, all tower plots will automatically be considered for litter sampling and then accepted according to the following criteria:

- 1) 1 or more individuals with DBH \geq 10 cm or;
- 2) 10 or more individuals with DBH \geq 5 cm

Plots that do not meet these criteria are not utilized for litter sampling.

Elevated traps

An elevated mesh litterfall trap (70.7 cm x 70.7 cm; 0.5 m², 0.8 m tall) will be placed at a random location within each plot/subplot, with trap locations selected from the herbaceous clip harvest list. Once set, traps will remain in the same location within the plot for sampling in subsequent years unless traps are removed for optimization. These traps will reliably sample shed leaves, needles, reproductive parts, and fine woody debris with butt-end diameter < 2 cm *and* length < 50 cm.. Traps will be sampled according the guidelines outlined in section 9 of this document. Deciduous forests will be sampled once in the spring then once every two weeks during leaf senescence. Evergreen systems including coniferous, xeric and tropical forests will be sampled year-round; the ideal sampling interval is every 4 weeks but may be extended to 8 weeks if dictated by logistical constraints.

In mixed woodland and grassland ecosystems (e.g. Domain 15 Onaqui, Domain 17 San Joaquin), woody vegetation cover is frequently patchy. As such, randomly placed litter traps are unlikely to adequately

| | | |
|------------------------------|------------------|----------------------|
| Title: | Author: K. Jones | Date: [Publish Date] |
| NEON Doc. #: NEON.DOC.001710 | | Revision: * |

capture litter dynamics from woody vegetation. In this case, NEON will target litter trap placement to randomly selected areas of the plot with woody cover, and then use remote sensing imagery from NEON’s Airborne Observation Platform (AOP) to estimate woody vegetation percent cover of the plot to scale litter production from the trap to the plot level. Scaling of this data will occur as part of the preparation of data products and is not expressly part of this protocol.

Ground traps

Ground traps for collecting large leaves, fronds, and fine woody debris with butt-end diameter < 2 cm and length > 50 cm, will be randomly located in plots at least 2 meters from elevated traps, consistent with Muller-Landau and Wright (2010). To avoid interfering with other sampling within the plot, the basic ground trap sampling unit will be one randomly selected 0.5 m x 3 m herbaceous clip harvest grid cell within the same plot or subplot as the elevated trap (Figure 1, SOP B). Ground traps are cleared of all relevant litter one year prior to the onset of sampling so that any litter within the selected area can be assumed to be the result of annual production. Only portions of large fronds or long sections of fine woody debris that lie inside the ground traps will be sampled; these sample locations will not move from year to year and will be excluded from consideration as locations for herbaceous clip harvest.

| | | |
|------------------------------|------------------|----------------------|
| Title: | Author: K. Jones | Date: [Publish Date] |
| NEON Doc. #: NEON.DOC.001710 | | Revision: * |

5 QUALITY ASSURANCE AND CONTROL

The procedures associated with this protocol will be audited according to the Field Audit Plan (RD[05]). Additional quality assurance will be performed on data collected via these procedures according to the NEON Data and Data Product Quality Assurance and Control Plan (RD[06]).

When unexpected field conditions require deviations from this protocol, the following field implementation guidance must be followed to ensure quality standards are met:

| Delay | Action | Adverse Outcome | Outcome for Data Product |
|---------------------|---|---|--|
| Hours | If delay prevents completion of litter collection from a single trap, resume collection as soon as possible. | None | None |
| | If delay occurs between plots, resume litter trap collection as soon as possible. | | |
| 1-7 days | If delay prevents completion of litter collection from a single trap <ol style="list-style-type: none"> 1. Store already collected litter in a cooler/refrigerator (okay), or sort and oven-dry as per protocol (best), 2. Resume collection of litter trap ASAP with new labeled bags 3. Combine dried biomass per functional group for weighing when all biomass is dry. | None | None |
| | If delay occurs between litter traps, resume collection of remaining litter traps as soon as possible. | | |
| 8-13 days or longer | If delay occurs between litter collection, resume harvest of next trap ASAP | Some litter mass may be lost from traps | More uncertainty in biomass and ANPP estimates |
| | If all traps are not collected in a single bout, prioritize collection of litter from missed traps at the subsequent bout | | |

Within a given year or growing season, Metcalfe et al. (2008) point out that litterfall collection efforts often have high levels of uncertainty and require greater sample size to accurately estimate annual production than other biomass pools. Additional traps may be installed at additional random (clip strip) locations per plot should variance of the litterfall estimate be greater than $\pm 10\%$ of the estimated mean based on analysis, conducted by Science Operations, of data from initial collection events (see RD[03] for details), and if technician labor is available.

| | | |
|-------------------------------------|-------------------------|-----------------------------|
| <i>Title:</i> | <i>Author:</i> K. Jones | <i>Date:</i> [Publish Date] |
| <i>NEON Doc. #:</i> NEON.DOC.001710 | | <i>Revision:</i> * |

If it is apparent that the volume of biomass collected from elevated and ground litter traps is too great to efficiently dry and process given limited drying oven space in the NEON domain laboratories, trap size or number may be reduced if justified based on sample optimization analysis conducted by Science Operations.

| | | |
|------------------------------|------------------|----------------------|
| Title: | Author: K. Jones | Date: [Publish Date] |
| NEON Doc. #: NEON.DOC.001710 | | Revision: * |

6 SAFETY

Personnel working at a NEON site must be compliant with safe field work practices as outlined in the Operations Field Safety and Security Plan (AD[02]) and EHS Safety Policy and Program Manual (AD[01]). Additional safety issues associated with this field procedure are outlined below. The Field Operations Manager and the Lead Field Technician have primary authority to stop work activities based on unsafe field conditions; however, all employees have the responsibility and right to stop their work in unsafe conditions.

A laser rangefinder/hypsometer/compass instrument is used to locate randomly assigned trap locations. Safety considerations for this instrument include:

- Avoid staring directly at the laser beam for prolonged periods. The rangefinder is classified as eye-safe to Class 1 limits, which means that virtually no hazard is associated with directly viewing the laser output under normal conditions. As with any laser device, however, reasonable precautions should be taken in its operation. It is recommended that you avoid staring into the transmit aperture while firing the laser.
- Never attempt to view the sun through the scope. Looking at the sun through the scope may permanently damage the eyes.

Pipe glue used to attach PVC legs to the elevated trap is highly flammable and may cause skin and eye irritation. Vapors are also potentially dangerous if inhaled. Technicians using glue should familiarize themselves with the hazards associated with this product (refer to the SDS), and with proper handling techniques.

Personnel assigned the task of constructing elevated traps shall attend Hand and Power Tool Safety Training and Machine Shop Safety. Personnel shall be trained in the safe use, maintenance and cleaning of the Wiley® Mill or equivalent.

| | | |
|-------------------------------------|-------------------------|-----------------------------|
| <i>Title:</i> | <i>Author:</i> K. Jones | <i>Date:</i> [Publish Date] |
| <i>NEON Doc. #:</i> NEON.DOC.001710 | | <i>Revision:</i> * |

7 PERSONNEL REQUIREMENTS

The lead plant technician must possess the demonstrated ability to identify collected plant structures to functional group via visual inspection. Preferably, the technicians sorting biomass are the same technicians who harvested the biomass in the field.

| | | |
|-------------------------------------|-------------------------|-----------------------------|
| <i>Title:</i> | <i>Author:</i> K. Jones | <i>Date:</i> [Publish Date] |
| <i>NEON Doc. #:</i> NEON.DOC.001710 | | <i>Revision:</i> * |

8 TRAINING REQUIREMENTS

All technicians must complete required safety training as defined in the NEON Training Plan (RD[04]). Additionally, technicians must complete protocol specific training for safety and implementation of protocol as required in Field Operations Job Instruction Training Plan (RD[05]).

Technicians must be proficient in the use of handheld GPS units in order to successfully navigate to plots for sampling.

| | | |
|------------------------------|------------------|----------------------|
| Title: | Author: K. Jones | Date: [Publish Date] |
| NEON Doc. #: NEON.DOC.001710 | | Revision: * |

9 SAMPLE FREQUENCY AND TIMING

The primary objective is to generate annual or per growing season estimates of litterfall and fine woody debris production within the dominant vegetation type (i.e. within Tower plots). Estimates of deciduous litterfall will be calculated on a per annum basis, with all of the litter produced in a given year contributing toward the yearly estimate. Evergreen litterfall estimates within a given calendar year do not necessarily reflect annual production due to the multi-year and somewhat variable lifespan of needles; however, the long-term average ($n =$ at least 3 years) will be used to estimate per annum needle production.

9.1 Sampling Frequency and Timing

Elevated traps

In predominantly deciduous systems with pronounced annual senescence, elevated litter traps will be sampled in the spring to account for winter production of fine woody debris, followed by biweekly sampling during the period of autumn senescence (Bernier et al. 2008). In systems dominated by plants that bear multi-year leaves or needles (e.g. D17 San Joaquin and D04 Guanica), elevated traps will be sampled throughout the year. Mixed forests with both evergreen and deciduous species will be sampled according to a hybrid approach; sampling should occur once a month with increased, bi-weekly sampling during senescence.

Litterfall in coniferous forests (e.g. D10 Rocky Mountain Park and D16 Wind River) or in xeric shrub systems (e.g. D14 Santa Rita and Jornada LTER) may be sampled with less frequency than deciduous broadleaf forests, but since there is no clear ‘litterfall season’ sampling will occur year round. NEON will sample litterfall in arid desert systems on a monthly basis (Table 2).

Once a month sampling is considered ideal to ensure data quality; however, sampling frequency at coniferous, xeric, tropical or mixed forest sites may be reduced to once every 8-weeks if dictated by logistical constraints.

Ground traps

Ground traps will be sampled annually in Tower plots.

9.2 Criteria for Determining Sampling Dates

Elevated trap sampling will vary depending on the vegetation present at a site (Table 2). Ground litter trap sampling will occur once a year and should occur within ± 2 weeks of the date on which sampling occurred the previous calendar year. Initiation of 2 week sampling intervals during leaf senescence may be determined by checking an elevated trap near the Tower; once litter material from falling leaves begins to accumulate in the trap, begin fall sampling. Data do not need to be collected on the ‘indicator

| | | |
|------------------------------|------------------|----------------------|
| Title: | Author: K. Jones | Date: [Publish Date] |
| NEON Doc. #: NEON.DOC.001710 | | Revision: * |

trap’ and the one selected for monitoring does not need to be recorded. The only stipulation is that the selected trap is surrounded by deciduous trees.

Table 2. Sample timing and frequency by vegetation type.

| Climate / Ecosystem | When to sample elevated traps |
|-----------------------------------|--|
| Temperate deciduous | <ul style="list-style-type: none"> - Once in the spring, approximately same time each year - Every two weeks during leaf senescence period |
| Coniferous / Evergreen / Tropical | <ul style="list-style-type: none"> - Once a month*, all year |
| Arid shrub | <ul style="list-style-type: none"> - Once a month*, all year |
| Mixed Deciduous/Evergreen | <ul style="list-style-type: none"> - Once a month* - Every two weeks during leaf senescence period |

* A 4 week sampling interval is ideal for purposes of data quality but may be decreased to once every 8-weeks if dictated by logistical constraints.

9.3 Sampling Frequency

Sampling frequency of elevated traps will vary based on the vegetation present at a site (Table 2). Ground traps will be sampled once a year.

9.4 Sampling Timing Parameters

Litter traps left full in the field for longer than the specified sampling interval may be subject to granivory by small mammals, herbivory by insects, or increased decomposition and resulting loss of mass. In deciduous forests, elevated traps must be checked at least every two weeks during leaf senescence, as traps may fill in relatively short periods. Collection of litter during leaf senescence may occur at intervals less than two weeks if litter volume is high and sufficient resources exist to support additional sampling; this is left to the discretion of the Domain manager and will not be dictated by Science Operations.

| | | |
|------------------------------|------------------|----------------------|
| Title: | Author: K. Jones | Date: [Publish Date] |
| NEON Doc. #: NEON.DOC.001710 | | Revision: * |

10 STANDARD OPERATING PROCEDURES

SOP A: Preparing for Sampling

1. Field Equipment and Materials

Table 3. Field Equipment List for SOP A.

| Maximo Item No. | Item Description | Quantity | Conditions Used | Action(s) |
|-----------------|---|-----------|--|---|
| Suggested | GPS unit | 1 | All | <ul style="list-style-type: none"> • Charge • Load target plot locations • Pack extra batteries |
| Suggested | Compass, mirror-sight | 1 | All | <ul style="list-style-type: none"> • Check/set correct declination¹ • May be used, in conjunction with less precise rangefinder as an alternative to TruPulse |
| MX100322 | TruPulse 360R laser rangefinder and clinometer | 1 | Finding correct trap location during trap deployment | <ul style="list-style-type: none"> • Check battery, charge (if possible) • Clean lenses with lens cloth or lens tissue (if necessary) • Check/set correct declination¹. See Appendix E for details. • Calibrate TruPulse tilt-sensor (only necessary after severe drop-shock; see Appendix E for details). |
| Suggested | Laser rangefinder, used for bird sampling | | Measuring distances | <ul style="list-style-type: none"> • May be used, in conjunction with handheld compass as an alternative to TruPulse |
| Required | Per plot or subplot Clip Lists ² (from RD[08]) | Variable | All | <ul style="list-style-type: none"> • Print on all-weather paper |
| Suggested | Random number list | 1 | Sites with targeted selection | <ul style="list-style-type: none"> • Generate randomized lists |
| Required | Datasheets for Litterfall and Fine Woody Debris (RD[12]) | As needed | All | <ul style="list-style-type: none"> • Print on all-weather paper |

¹ Declination changes with time and should be looked up annually per site:

<http://www.ngdc.noaa.gov/geomag-web/>

² Provided separately by Science Operations on request once plot establishment has been completed.

| | | |
|-------------------------------------|-------------------------|-----------------------------|
| <i>Title:</i> | <i>Author:</i> K. Jones | <i>Date:</i> [Publish Date] |
| <i>NEON Doc. #:</i> NEON.DOC.001710 | | <i>Revision:</i> * |

2. Gather necessary resources for field work

- 1) Print clip strip lists for the plots that will be visited
 - Litterfall sampling locations will be selected from the plot-specific randomized lists created for herbaceous clip harvest locations RD[08]. These lists are therefore essential for the completion of the trap deployment procedure (SOP B), and must be updated to reflect the fact that two of the clipID locations are occupied by litter traps (elevated and ground). For the purpose of this protocol, trap location and clipID are used interchangeably.
 - Make sure that all fields in the clip strip lists are up to date, that clip strips that have been harvested or rejected are current and indicated on the lists
- 2) Gather all field equipment
- 3) Load plot locations into GPS unit

| | | |
|------------------------------|------------------|----------------------|
| Title: | Author: K. Jones | Date: [Publish Date] |
| NEON Doc. #: NEON.DOC.001710 | | Revision: * |

SOP B: Field Sampling – Trap Deployment

1. Field Equipment and Materials

Table 4. Field Equipment List for trap deployment

| Maximo Item No. | Item Description ¹ | Qty | Conditions Used | Purpose |
|-----------------|---|------------|---------------------|---|
| | Elevated trap kits (NEON.DOC.001813) | 40-50 | All | Construct elevated traps |
| Required | PVC pipe cutter | 1 | All | Cut PVC as needed |
| Required | Pipe glue | 1 jar | | Permanently attach PVC from the elevated trap kits |
| Required | Bubble Level ~20 cm (e.g. “torpedo” or “carpenters” level) | 1 | All | To check the angle of the elevated trap |
| Required | Brightly colored Ground trap markers – PVC or non-oxidizable metal | 4 per trap | All | Identify ground trap area |
| Required | Non-oxidizable metal rods (e.g. aluminum, galvanized steel, or equivalent) ~1 m length ² | 4 per trap | All | Anchor trap to sampling location |
| Required | Per plot or subplot Clip Lists ³ (from RD[08]) | | All | Print on all-weather paper |
| MX100322 | TruPulse 360R laser rangefinder and clinometer | 1 | All | Used to locate X, Y coordinates of within-plot trap location |
| MX103218 | Foliage filter for laser rangefinder | 2 | Brushy vegetation | Facilitates use of TruPulse in very brushy conditions. |
| Suggested | Reflective surface (3-in white reflector or reflective tape on back of field notebook/clipboard) | 1 | Used with TruPulse | Aids in accurate location of clip-harvest strips with TruPulse in “FLT” mode, particularly in brushy vegetation. |
| Required | Extra battery for TruPulse (CR123A type) | 2 | Used with TruPulse | Battery backup |
| Suggested | Laser rangefinder, used for bird sampling | | Measuring distances | May be used, in conjunction with handheld compass as an alternative to TruPulse |
| Suggested | Compass, mirror-sight | 1 | All | Check/set correct declination ¹ May be used, in conjunction with less precise rangefinder as an alternative to TruPulse |
| MX104361 | Chaining pins, steel | 2 | All | Stretching tapes, plot boundary delineation |
| Required | Fiberglass meter tape (30m) | 1 | Plot slope < | Locate clip-harvest strips within |

| | | |
|-------------------------------------|-------------------------|-----------------------------|
| <i>Title:</i> | <i>Author:</i> K. Jones | <i>Date:</i> [Publish Date] |
| <i>NEON Doc. #:</i> NEON.DOC.001710 | | <i>Revision:</i> * |

| | | | | |
|-----------|--|---------------|-------------------------------------|---|
| | or longer) | | 10 deg; grassland, savannah | plots/subplots. |
| Suggested | Coin | 1 | Sites with targeted selection | Used to randomize selection of patches |
| Suggested | Random number list | 1 | Sites with targeted selection | Used to randomize selection of patches |
| Required | Datasheets for Litterfall and Fine Woody Debris | Vari- able | All | Record required data and metadata |

¹All permanent marker material and color selection is contingent on approval by the NEON site host or local landmanager

² 1 meter is ideal but may be adjusted as needed to suit site conditions³ Provided separately by Science Operations on request once plot establishment has been completed.

2. Selecting litter trap location strategy

Litter traps will be deployed in pairs, one elevated and one ground trap per pair. There will be one set of paired traps for every 400 m² plot/subplot area. Because litter sampling will primarily occur in forested sites where plot size is typically 1600 m² or more, most plots will have at least four pairs of traps. Refer to the TOS Protocol and Procedure: Plot Establishment RD[09] for details on handling measuring tapes and plot delineation tips.

- 1) Navigate to the desired plot.
- 2) Determine whether targeted or random selection of litter trap location is required. Refer to Appendix C for general guidance. Trap location strategy is based on NLCD vegetation classification, select strategy based on the conditions of the plot, even if they differ from
 - **Targeted selection** – for patchy vegetation, where overstory species ≥ 2 m height is present throughout $< 50\%$ of the plot area.
 - **Random selection** – for forested sites with relatively continuous canopy

3. Locating targeted elevated trap location

- 1) Assess location of patches within the plot or subplot (depending on plot size)
- 2) Give each patch a numeric value. Assign values sequentially, left to right, bottom to top, beginning in the SW corner (Figure 1)
- 3) Use either a random number list or a series of coin flips to randomly select a patch to target for litterfall and fine woody debris sampling.
- 4) Once a patch is selected, select a location under the canopy, central to the patch to place an elevated litter trap.
- 5) Use the range finder to measure the distance to plot/subplot edges.
- 6) Determine where the nearest clip strip centroid is located.

| | | |
|------------------------------|------------------|----------------------|
| Title: | Author: K. Jones | Date: [Publish Date] |
| NEON Doc. #: NEON.DOC.001710 | | Revision: * |

- 7) If practical, center trap over that point, this will minimize the number of clips that will be removed from consideration for herbaceous clip harvest.
 - In the example provided in Figure 1, the coordinates associated with nearest clip strip centroid from the center of patch 4 are, $x = 3.7$, $y = 11.5$.
 - Not centering the trap over a centroid is acceptable but not ideal as there will be more cells excluded from consideration for herbaceous clip harvest.
- 8) Place a pin flag at the selected trap location.

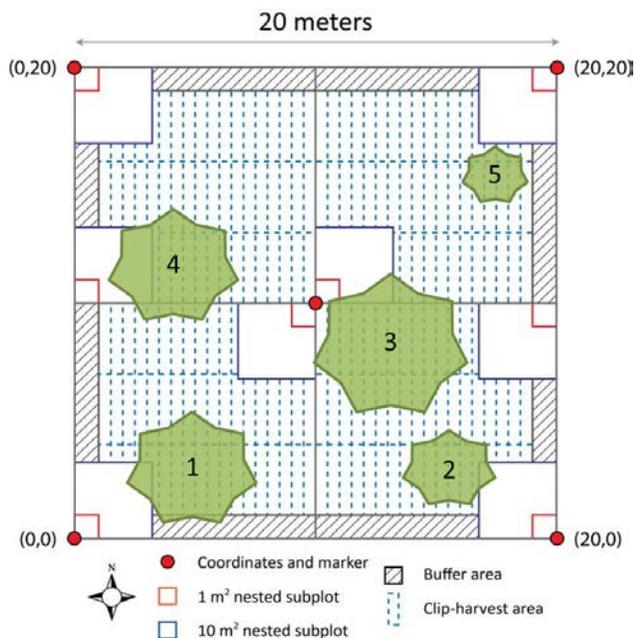


Figure 1. Example of numbering system for qualifying patches of vegetation within a plot

4. Locating random elevated trap location

Use the plot- or subplot-specific Clip List ([plotID]_clipList.csv) to identify the first potential clip-strip location that has not already been sampled or rejected. Where relevant, subplot number is included in the file name and is also provided as a field in the spreadsheet.

- 1) Navigate to the SW corner of the desired clipID:

| | | |
|------------------------------|------------------|----------------------|
| Title: | Author: K. Jones | Date: [Publish Date] |
| NEON Doc. #: NEON.DOC.001710 | | Revision: * |

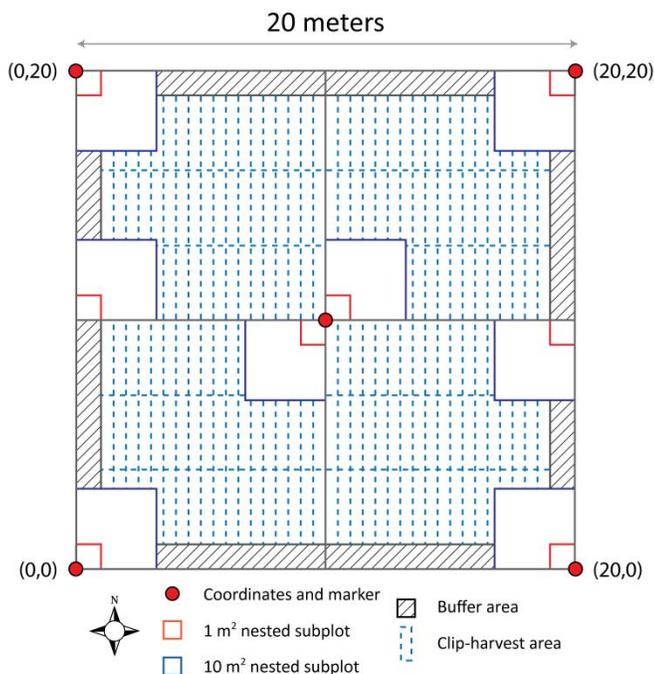


Figure 2. A 20 m x 20 m NEON plot) showing the locations of 0.5m x 3m clip-harvest “cells” (dashed blue lines). Larger plots will have different nested subplots, but the coordinate numbering system for the 20 m subplot within these plots will follow the same conventions as shown above.

If the Y-coordinate is < 10:

- a) Run a tape East/West along the south edge of the plot or subplot between the (0,0) → (20,0) plot markers (Figure 1), and stretch the tape taut.
- b) Place a pin flag at the desired relative X-coordinate.
- c) Standing directly over the pin flag that was just placed at the X-coordinate, use the TruPulse in **HD** mode with a reflective surface to locate the Y-coordinate.
 - Make sure the azimuth is 0° (True North) when shooting the TruPulse to find the Y-coordinate (see Appendix E).
 - Note: if TruPulse is not available, the same routine described here may be completed using a handheld compass to verify azimuth and a laser rangefinder or additional tape measure for distance.
- d) Place a pin flag at the clip-strip (X,Y) location.

If the Y-coordinate is > 10:

- a) Run a tape East/West from the plot/subplot centroid (10,10) to either the (0,10) position or the (20,10) position (Figure 1):

| | | |
|------------------------------|------------------|----------------------|
| Title: | Author: K. Jones | Date: [Publish Date] |
| NEON Doc. #: NEON.DOC.001710 | | Revision: * |

| X-coordinate | Tape Layout ¹ |
|--------------|--------------------------------------|
| 1 < X < 10 | From (10,10) to (0,10) ¹ |
| 10 < X < 20 | From (10,10) to (20,10) ¹ |

¹ Use the TruPulse in **AZ** mode to guide the tape along the correct azimuth

- b) Place a pin flag at the desired relative X-coordinate.
- c) Standing directly over the pin flag that was just placed at the X-coordinate, use the TruPulse in **HD** mode with a reflective surface to locate the Y-coordinate.
 - Make sure the azimuth is 0° (True North) when shooting the TruPulse to find the Y-coordinate (see Appendix E).
 - Note: if TruPulse is not available, the same routine described here may be completed using a handheld compass to verify azimuth and a laser rangefinder or additional tape measure for distance.
- d) Place a pin flag at the clip-strip (X,Y) location.

BEST PRACTICE TIPS

- Use the TruPulse laser rangefinder in **HD** mode to place the initial pin flags if the plot slope is > 10 %, or there is significant brush or obstacles that prevent accurately stretching a tape.
 - Plot slope can be quickly estimated using the inclinometer in the TruPulse (**INC** mode) or the inclinometer on the handheld compass.
- 2) Assess the suitability of the strip for an elevated litter trap:
 - Accept the strip if there is a canopy formed by woody vegetation, directly overhanging the strip.
 - If the strip is not acceptable for placement of an elevated litter trap, move to the next strip on the list but do NOT record the strip status as rejected for herbaceous biomass sampling.
 - 3) Navigate to center of the strip (1.5 m north, 0.25 m east), place a pin flag. Elevated traps will be centered over this point.
 - If there is no vegetation directly overhanging the litter trap at strip center, the trap may be shifted up to 1 meter North or South to a location where litter falling in a straight line from the canopy will be intercepted by the trap.
 - Record clip-strip as selected for litter on the Clip List sheet but this does not need to be reported with the clip harvest data.

| | | |
|------------------------------|------------------|----------------------|
| Title: | Author: K. Jones | Date: [Publish Date] |
| NEON Doc. #: NEON.DOC.001710 | | Revision: * |

5. Locating ground trap clip strip

- 1) Using the same procedure described above, in subsections 3 and 4, select an appropriate location for the ground trap
 - **Targeted selection**– repeat the process for randomly selecting a patch in which to locate the ground trap. Do not exclude the patch selected for the elevated trap from consideration. The ground trap location does need to be within a single clip strip cell.
 - **Random selection**- continue using the randomized clip strip locations in sequential order, assess the suitability of the next potential clip-strip location that has not previously been sampled or rejected.
 - Reject the trap location if the selected strip is < 2 meters from the elevated trap
- 2) Delineate the 3 m x 0.5 m clip strip that will be used for the ground trap using meter tape and compass or TruPulse to ensure that the trap is oriented to the cardinal directions.
- 3) Hammer in brightly colored stakes in each of the four corners leaving ~20cm visible above ground.
- 4) Remove all large leaves, large fronds, and ALL fine woody debris from within the ground trap area.
 - It is not necessary to remove small leaves, fronds, etc. that are normally sampled with the elevated litter traps.

5. Elevated trap construction and installation

- 1) Center square trap frame over pin flag placed in the center of the selected clip strip cell
- 2) Mark plot corners with pin flags
 - The trap frame is 70.7 cm wide, since a clip strip cell is 50 cm wide, trap legs will be anchored 10 cm into the adjoining cells on either side of the selected cell
- 3) Hammer non-oxidizable metal stakes into ground at the pin flag locations to anchor trap legs, leaving 50 cm above ground
- 4) Attach trap legs to square frame, glue in place
- 5) Cut the trap legs so that, once installed, the square frame is level (use bubble level to check), approximately 0.8 m above the ground.
- 6) Slide trap legs over stakes.

| | | |
|-------------------------------------|-------------------------|-----------------------------|
| <i>Title:</i> | <i>Author:</i> K. Jones | <i>Date:</i> [Publish Date] |
| <i>NEON Doc. #:</i> NEON.DOC.001710 | | <i>Revision:</i> * |

- 7) Attach screen to square frame with the provided zip ties (Figure 3).
 - The pre-cut screen is larger than the trap area and should not be taut across the trap, some sag is necessary to prevent litterfall from blowing away.
- 8) Record tagIDs of individuals overhanging the trap on the “Trap Deployment Datasheet” (RD [12]).



Figure 3. Fully constructed elevated litter trap, NEON traps will have legs attached on corners rather than center (photo from Muller-Landau and Wright 2010).

| | | |
|------------------------------|------------------|----------------------|
| Title: | Author: K. Jones | Date: [Publish Date] |
| NEON Doc. #: NEON.DOC.001710 | | Revision: * |

SOP C: Field Sampling

1. Field Equipment and Materials

Table 5. Equipment list for Field Sampling of elevated and ground litter traps.

| Maximo Item No. | Item Description | Quantity | Conditions Used | Purpose |
|-----------------------|--|-----------------|--------------------|---|
| MX100322 | TruPulse 360R laser rangefinder | 1 | Thick brush | Used to locate X, Y coordinates of trap if thick brush prevents visual trap location. |
| MX103218 | Foliage filter for laser rangefinder | 2 | Brushy vegetation | Facilitates use of TruPulse in very brushy conditions. |
| Suggested | Extra battery for TruPulse (CR123A type) | 2 | Used with TruPulse | Battery backup |
| Required | Cloth bags, two colors, numbered and marked with an E or G (for Elevated or Ground trap identification)* | 2 per trap pair | All | Storage and transport of fresh, potentially wet, litter samples. |
| Suggested | Heavy duty clippers | 1 | | For cutting branches up to 2 cm diameter |
| Suggested | Measuring stick† | 1 | | Quick measurement of 50cm |
| Required | Bubble Level ~20 cm (e.g. "torpedo" or "carpenters" level) | 1 | All | To check the angle of the elevated trap |
| Required | Calipers | 1 | All | Measure branch diameters |
| Suggested | Window screen patch kit (small pieces of screen, wire, wirecutters) | 1 | | For repairing minor holes in screen material |
| Required - EB07670000 | Elevated trap kits | 2 | All | Replace damaged traps |
| Suggested | Replacement stakes for ground traps | 4 | All | Replace damaged ground traps |
| Required | General Purpose Manila Tags, Pre-strung, 4-3/4" x 2-3/8" | 2 per trap pair | All | Label collection bags |
| Required | Nylon cord | 1, 8 m | All | Delineate ground trap |

* <http://www.statelinebagwholesale.com/store/p/40-12-x-20-Premium-Single-Drawstring-Cotton-Muslin-Bags-100-Count.aspx> or <http://muslinbag.com/import.html> or similar.

† May also mark 50cm on plot frame with permanent marker.

| | | |
|------------------------------|------------------|----------------------|
| Title: | Author: K. Jones | Date: [Publish Date] |
| NEON Doc. #: NEON.DOC.001710 | | Revision: * |

2. Fine litter collection – Elevated traps

- 1) Navigate to plot
- 2) Assess and record the **trapCondition** (Table 6)

Table 6. Prescribed “trapCondition” codes.

| Code | Description |
|------|---|
| 1 | Litter collected - Trap in good shape, no issues |
| 2 | Litter not collected – Trap empty |
| 3 | Litter not collected - Holes large enough for leaves to pass through. Holes near the base of the screen (the lowest hanging point) are worse than holes on the side of the screen. |
| 4 | Litter not collected – trap blocked. Large branches or leaves (especially palm fronds) present in the trap which may have prevented trap from collecting litter or diverted falling litter away from the trap |
| 5 | Litter not collected – trap tilted $\geq 10^\circ$ (use clinometer on compass to measure) |
| 6 | Litter not collected – trap broken, requires replacement |

- 3) If the trap is not in good condition (3-6), discard the litter and make necessary repairs. Broken traps should be replaced immediately if possible.
- 4) If the trap is in good condition (1) continue with collection procedure.
- 5) Discard litter > 50 cm in length, this material is not reliably collected in the elevated traps and will be sampled in ground traps
- 6) All woody material > 2 cm diameter will be measured according to the Coarse Wood Debris (CWD) protocol. Use calipers to measure diameter of woody branches
 - a. Discard branches > 2 cm at narrowest point
 - b. For branches that taper to ≤ 2 cm, cut off and discard the portion > 2 cm diameter, discarded portion of branches may be dropped, haphazardly (i.e. do not group or stack discarded material), beside the elevated litter trap
- 7) Transfer all other material, including parts hanging out of the trap, into the cloth bag designated for elevated trap litter
- 8) Create label with clipID, date, trap type, and technicianID (Figure 3Figure 3), and attach to bag.




Figure 4. Example field collection label.

| | | |
|------------------------------|------------------|----------------------|
| Title: | Author: K. Jones | Date: [Publish Date] |
| NEON Doc. #: NEON.DOC.001710 | | Revision: * |

- 9) Knot cloth bag to prevent material from falling out while in transport, do not use draw strings if present on bags
- 10) Record remarks if necessary.

3. Woody litter collection - Ground

- 1) Locate stakes marking ground trap location
- 2) Assess and record **trapCondition** (Table 7)

Table 7. Modified trapCondition codes for ground traps.

| Code | Description |
|------|--|
| 1 | Litter collected - Trap in good shape, no issues |
| 2 | Litter not collected – trap blocked. Large branches or tree > 10 cm diameter have fallen over trap which may have diverted falling litter away from the trap |

- If trap condition is blocked (code=2), do not collect. If obstruction cannot be cleared, move ground trap to a new location from the clip strip list.
 - i. Record the new trap location/clip strip ID in the **trapMoved** field
 - ii. Clear all litter from the new strip
 - iii. Do not collect
- 3) Wrap nylon cord around the four staked corners of the ground trap, delineating the trap edges.
 - 4) Identify qualifying litter which is:
 - > 50 cm length and
 - < 2 cm diameter
 - 5) Cut off and discard portions of qualifying litter which overhang the trap edges even if this means creating pieces < 50 cm in length.
 - 6) Cut off and discard portions of woody branches > 2 cm diameter
 - 7) Collect all remaining qualifying litter from within the ground trap, transfer material to the cloth bag designated for ground trap litter
 - Pieces may be cut to smaller lengths if they are too long to fit in the cloth collection bags.
 - 8) Create label with clipID, date, trap type, technicianID (Figure 3), and attach to bag.
 - 9) Knot cloth bag to prevent material from falling out while in transport, do not use draw strings if present on bags
 - 10) Record remarks if necessary.

| | | |
|-------------------------------------|-------------------------|-----------------------------|
| <i>Title:</i> | <i>Author:</i> K. Jones | <i>Date:</i> [Publish Date] |
| <i>NEON Doc. #:</i> NEON.DOC.001710 | | <i>Revision:</i> * |

SOP D: Laboratory Processing and Analyses

1. Laboratory Equipment and Materials

Table 8. Laboratory Equipment List for SOP D.

| Maximo Item No. | Item Description | Qty | Conditions Used | Purpose |
|------------------------|---|----------------|--|---|
| Suggested | Large plastic bag (black trash bag or equivalent); e.g. Uline # S-5111 | Box of 100 | All | Temporary storage of oven dried samples before they are weighed |
| Required | Sample microsplitter (small capacity) | 1 | Relatively little litter mass per biomassCode per trap | Creates identical sub-samples from relatively small volumes of ground sample |
| Required | Sample splitter (large capacity) | 1 | Relatively large litter mass per biomassCode per trap | <ul style="list-style-type: none"> Creates identical sub-samples from relatively large volumes of ground sample Useful with fibrous leaves. |
| Required | Hi-back pans for sample splitter (sized to match splitter size) | 2 per splitter | All | Receives sub-samples generated by splitter |
| Required | 20 mL Scintillation vials with caps | As needed | All | Containers for storing ground split samples for shipment to archive or chemical analysis |
| Required | Paper bags, 8# kraft or similar | 50 | All | Temporary storage of litter, sorted to functional group |
| Required | Datasheets: <ul style="list-style-type: none"> Lab Drying QC Datasheet Lab Weighing Datasheet | As needed | All | Recording dry weight of herbaceous biomass |

| | | |
|------------------------------|------------------|----------------------|
| Title: | Author: K. Jones | Date: [Publish Date] |
| NEON Doc. #: NEON.DOC.001710 | | Revision: * |

2. Laboratory processing

- 1) If litter and bags are very wet (i.e. dripping), hang bags to air dry before further processing.
- 2) Sort litter from each “E” and “G” bag per trap to functional group.
 - a. Clear adequate bench space in the laboratory.
 - b. Empty the a cloth bag filled with litter onto the bench, and sort litter pieces to the functional groups in Table 9 (“E” bags) or Table 10 (“G” bags).

Table 9. Elevated trap litter functional group codes

| biomassCode | Description |
|-------------|--|
| ELVS | Leaves (including petioles, rachis and non-woody tendrils) |
| ENDL | Needles from coniferous species |
| ETWI | Twigs/branches < 2 cm diameter <i>and</i> < 50 cm length |
| EWDY | Woody material (e.g. bark, cones, etc.) |
| ESDS | Seeds |
| EFLR | Flowers (including pedicels) |
| EOTR | Other (lichen, mosses, unidentifiable material, etc.) |

Table 10. Ground trap litter functional group codes

| biomassCode | Description |
|-------------|---|
| GLVS | Leaves and needles > 50 cm length (including petioles, rachis and non-woody tendrils) |
| GTWI | Twigs/branches < 2 cm diameter <i>and</i> > 50 cm length |

- 3) Label paper bags to hold sorted litter functional groups from each trap. Include sampling information from tag on cloth bag, as well as the appropriate litter “biomassCode”.
 - a. For each cloth “E” bag, label 7 paper bags. Choose either 8# or 25# kraft bags, depending on the quantity of litter.
 - b. For each cloth “G” bag, label 2 paper bags. Again, choose bag size depending on the quantity of litter.
- 4) Label the time (24 hr time, e.g. 1645 for 4:45 pm) and date (YYYYMMDD) that bags are placed in the drying oven on the back side of the tag.
 - a. **Critical step:** Labeling bags allows assessment of how long different batches of bags have been in the oven, especially when harvests from multiple days occupy the same oven. Additionally, organizing the oven by grouping samples from a given day in the same area will streamline the re-measurement process; 48-hour samples may be located and removed for weighing without requiring a complete unloading of the contents of the oven.
- 5) Place bags of litter (excluding ETWI, EWDY and GTWI) in a drying oven set to 65° C for 48h – 120h (2d – 5d), until constant mass is attained.

| | | |
|------------------------------|------------------|----------------------|
| Title: | Author: K. Jones | Date: [Publish Date] |
| NEON Doc. #: NEON.DOC.001710 | | Revision: * |

- 6) Check the drying progress of litter bags using the “Lab Drying QC” datasheet.
 - a. Check the weight of the same subset of n=10 bags per date after day 1, 2, 3, etc.
 - b. Calculate the difference in weight between the latest two time points for each bag.
 - c. Samples are dry when the average weight difference between the latest two timepoints = 0 (averaged across all n=10 bags, ± 0.05 g or 1%, whichever is greater)
- 7) Clean off any dirt attached to litter from ground traps.
- 8) Place bags of ETWI, EWDY and GTWI litter in a drying oven set to 101-105° C for 24-72 hours, until constant mass is attained. If multiple drying ovens are available, steps 5-6 and 8-9 may be occur simultaneously, otherwise, complete drying of litter material at 65° C before increasing the temperature to dry FWD. Woody material requires higher drying temperatures to release bound water.
- 9) Check the drying progress of litter bags using the “Lab Drying QC” datasheet.
 - a. Check the weight of the same subset of n=10 bags per date after day 1, 2, 3, etc.
 - b. Calculate the difference in weight between the latest two time points for each bag.
 - c. Samples are dry when the average weight difference between the latest two timepoints = 0 (averaged across all n=10 bags, ± 0.05 g or 1%, whichever is greater)
- 10) Store sorted material in labeled paper bags (8# or 25# kraft bags, or similar), inside a larger, sealed, plastic bag (e.g. a black plastic garbage bag or equivalent). Placing samples in a bag is important as paper bags and dried samples may absorb water from the air as they cool, particularly in humid environments. Once dried and sealed in a bag, samples may be stored indefinitely prior to weighing.
 - a.
- 11) Weigh material from each functional group on mass balance (0.01g accuracy).
- 12) Record the mass to the nearest 0.01g on the “Litter Weight” datasheet. For large volumes of biomass that do not readily fit into a large weigh boat, use any of the following strategies:
 - Use a paper bag or a large cardboard box lid (or equivalent) instead of a weigh boat.
 - Crush or chop the biomass to reduce volume so it will fit into a weigh boat.
 - *Avoid splitting the biomass into subgroups for weighing, as uncertainty values must be added each time a subgroup is created.*
- 13) Once all weights have been recorded, return biomass to the large plastic bag, seal, and place in temporary storage. Samples in temporary storage can then be prepared as time permits for bioarchive and chemical analysis.

| | | |
|------------------------------|------------------|----------------------|
| Title: | Author: K. Jones | Date: [Publish Date] |
| NEON Doc. #: NEON.DOC.001710 | | Revision: * |

3. Grinding dried litter for archive and chemical analysis

Select samples from one trap per plot from one collection event per year to submit for bioarchive and chemical analysis. In coniferous evergreen systems, collect a sample for archive from the October collection event broadleaf evergreen vegetation (including tropical sites) may likewise ground and archived in October. In deciduous and mixed forest systems, select a sample from the period of peak senescence, this date may vary from site to site and from year to year, . Refer to the site specific appendix D for suggested sampling windows, use assessment of local conditions to ultimately drive this decision.

- 1) Coarsely grind each functional group per clipID (trap) with a Wiley Mill (0.85mm, 20 mesh size).
- 2) Use an appropriately sized splitter/microsplitter to generate two representative sub-samples of approximately 20 mL volume:
 - Sample 1: Bioarchive sample
 - Sample 2: Chemical analysis sample
 - Note : In order to meet data product requirements, NEON must provide chemical analysis of litter material therefore this sample, Sample 2, is the priority. If total ground material is <0.5g, only fill the chemical analysis sample vial.

BEST PRACTICE TIPS

- If the split sub-sample is too large to fit into the vial in its entirety, continue splitting until a sub-sample of the desired size is generated.
 - DO NOT create sub-samples with a scoopula or spatula. These tools should only be used to transfer an ENTIRE sub-sample into a vial.
- 3) Place the split sub-samples into 20 mL polypropylene scint vials, and label the vials with:
 - a. date
 - b. clipID
 - c. Functional group code (i.e. biomassCode)

| | | |
|------------------------------|------------------|----------------------|
| Title: | Author: K. Jones | Date: [Publish Date] |
| NEON Doc. #: NEON.DOC.001710 | | Revision: * |

SOP E: Data Entry and Verification

Following the completion of each field or lab data sampling bout, all data recorded manually on datasheets must be entered electronically in the provided MS Access database and saved to the NEON server. Any questions that arise while in the field should be answered as soon as possible to avoid losing information.

The data ingest document contains at least the following spreadsheets:

- **ltrFieldSummary_in**: Spreadsheet summarizing each data ingest table, and defining table field names and ingest rules.
- **ltr_pertrap_in**: Metadata describing trap placement
- **ltr_fielddata_in**: Metadata describing individual sampling events on a per trap per plotID per sampling date basis.
- **ltr_labdata_in**: Oven-dried biomass data for each functional group per clipID per eventDate, as well as weighing QA data.

1. Entering and Uploading Field Data

- 1) For data collected on paper datasheets: Transcribe data into appropriate MS Access “litter” database template in accordance with data entry and data QA/QC protocols (RD[06]).
- 2) Data entry fields mirror the datasheet, do not change formatting on the provided spreadsheet.
- 3) Example entries of each data field are provided in the ‘ltrFieldSummary_in’ tab of the ‘litterfall and fine woody debris’ ingest workbook (RD [11]) or the ‘ltrFieldSummary’ tab of the ‘ltr_dataIngest_2014’ MS Access database. Consult this table for appropriate values and formats for each field in the subsequent worksheets.
- 4) If this is the first bout at a site or a trap had to be moved to a new clipID, transcribe data from the ‘SOP B: Trap Deployment’ Datasheets to the “ltr_pertrap_in” ingest table.
- 5) For collection events, record metadata for date, trapCondition and bags used in the ‘ltr_fielddata_in’. If the trapMoved field has a new clipID location, make sure that this is also captured in the ‘ltr_pertrap_in’.
- 6) Following completion of lab processing, record the weights of each functional group in the ‘ltr_labdata_in’ ingest table.
- 7) Update permanent digital versions of the “clip-strip coordinate” lists with “date” and “status” data recorded in the field.
- 8) Lab Drying QC data are not transcribed for ingest into the NEON CYI.
- 9) Once all data from the most recent sampling bout have been collected and transcribed, save only the data from the most recent bout to a .csv file for ingest by NEON CYI.
- 10) For data collected on the NEON digital data collection device: Download all data according to the protocols for data handling. Address any QA/QC concerns.

| | | |
|-------------------------------------|-------------------------|-----------------------------|
| <i>Title:</i> | <i>Author:</i> K. Jones | <i>Date:</i> [Publish Date] |
| <i>NEON Doc. #:</i> NEON.DOC.001710 | | <i>Revision:</i> * |

2. Equipment Maintenance, Cleaning and Storage

- 1) Charge/replace TruPulse batteries, if necessary.
- 2) Charge GPS unit.
- 3) Clean grinding mill and splitters.

| | | |
|------------------------------|------------------|----------------------|
| Title: | Author: K. Jones | Date: [Publish Date] |
| NEON Doc. #: NEON.DOC.001710 | | Revision: * |

11 REFERENCES

- Bernier, P., P. J. Hanson, and P. S. Curtis. 2008. Measuring litterfall and branchfall. Pages 91-101 *in* C. M. Hoover, editor. Field measurements for forest carbon monitoring. Springer, New York.
- Clark, D. A., S. Brown, D. W. Kicklighter, J. Q. Chambers, J. R. Thomlinson, and J. Ni. 2001. Measuring net primary production in forests: Concepts and field methods. *Ecological Applications* **11**:356-370.
- Metcalfe, D., P. Meir, L. E. O. C. Aragão, A. da Costa, S. Almeida, A. Braga, P. Gonçalves, J. Athaydes, Y. Malhi, and M. Williams. 2008. Sample sizes for estimating key ecosystem characteristics in a tropical *terra firme* rainforest. *Forest Ecology and Management* **255**:558-566.
- Muller-Landau, H., and S. J. Wright. 2010. Litterfall monitoring protocol. CTFS Global Forest Carbon Research Initiative:1-16.
- Williamson, G. B., and M. C. Wiemann. 2010. Measuring wood specific gravity...Correctly. *American Journal of Botany* **97**:519-524.

| | | |
|-------------------------------------|-------------------------|-----------------------------|
| <i>Title:</i> | <i>Author:</i> K. Jones | <i>Date:</i> [Publish Date] |
| <i>NEON Doc. #:</i> NEON.DOC.001710 | | <i>Revision:</i> * |

APPENDIX A

QUICK REFERENCES

| | | |
|-------------------------------------|-------------------------|-----------------------------|
| <i>Title:</i> | <i>Author:</i> K. Jones | <i>Date:</i> [Publish Date] |
| <i>NEON Doc. #:</i> NEON.DOC.001710 | | <i>Revision:</i> * |

APPENDIX B

CHECKLISTS

| | | |
|-------------------------------------|-------------------------|-----------------------------|
| <i>Title:</i> | <i>Author:</i> K. Jones | <i>Date:</i> [Publish Date] |
| <i>NEON Doc. #:</i> NEON.DOC.001710 | | <i>Revision:</i> * |

APPENDIX C SITE SPECIFIC CONSIDERATIONS

Burning – litter will need to be collected and traps removed before planned management activities, then replaced soon after.

| | | |
|------------------------------|------------------|----------------------|
| Title: | Author: K. Jones | Date: [Publish Date] |
| NEON Doc. #: NEON.DOC.001710 | | Revision: * |

APPENDIX D SITE SPECIFIC SAMPLING DATES

The dates listed here are estimated by MODIS averaged EVI values from 2001-2009 and are the ‘average Greenness Increase’ date a proxy for the beginning of spring, the time period when sampling for winter litterfall, and the beginning and average end of senescence. As the priority for litter sampling is on the Tower plots the sampling dates in this table are based on MODIS data for an area centered on the NEON flux tower; NLCD vegetation classification listed is based on the dominant vegetation found in the tower airshed. Sampling schedules may be modified based on local conditions, for example, if the NLCD vegetation class is identified as ‘Mixed Forest’ but plots are almost entirely coniferous trees, sampling may be shifted to ‘Monthly, Year Round’ even though the table specified ‘Spring + Senescence’ sampling schedule. Dates are only listed for sites with forests where intensive sampling during fall senescence is anticipated; all other sites will be sampled once a month all year or not at all.

| Domain | Site code | primary airshed NLCD | Trap Location Selection | Suggested Sampling Schedule | Average Greenness Increase | Beginning of Senescence | Average End of Senescence |
|--------|-------------|------------------------------|-------------------------|-----------------------------|----------------------------|-------------------------|---------------------------|
| 1 | BART | Mixed Forest | Random | Spring + Senescence | 120 | 220 | 300 |
| 1 | SAWB | Deciduous Forest | Random | Spring + Senescence | 110 | 220 | 315 |
| 1 | HARV | Mixed Forest | Random | Spring + Senescence | 110 | 220 | 300 |
| 2 | BLAN | DeciduousForest / PastureHay | Targeted | Spring + Senescence | 75 | 210 | 310 |
| 2 | SCBI | Deciduous Forest | Random | Spring + Senescence | 85 | 150 | 320 |
| 2 | SERC | Deciduous Forest | Random | Spring + Senescence | 80 | 220 | 325 |
| 3 | DSNY | Grassland Herbaceous | | None | | | |
| 3 | JERC | #N/A | | | | | |
| 3 | OSBS | #N/A | | Monthly, Year Round | | | |
| 4 | GUAN | Evergreen Forest | Random | Monthly, Year Round | | | |
| 4 | LAJA | Cultivated Crops | | None | | | |
| 4 | MAME | Evergreen Forest | Random | Monthly, Year Round | | | |
| 5 | STEI | Deciduous Forest* | Random | Spring + Senescence | 120 | 215 | 250 |
| 5 | TREE | Deciduous Forest | Random | Spring + Senescence | 120 | 215 | 250 |

| | | |
|------------------------------|------------------|----------------------|
| Title: | Author: K. Jones | Date: [Publish Date] |
| NEON Doc. #: NEON.DOC.001710 | | Revision: * |

| Domain | Site code | primary airshed NLCD | Trap Location Selection | Suggested Sampling Schedule | Average Greenness Increase | Beginning of Senescence | Average End of Senescence |
|--------|-------------|----------------------|-------------------------|-----------------------------|----------------------------|-------------------------|---------------------------|
| 5 | UNDE | Woody Wetlands | Targeted | Spring + Senescence | 125 | 215 | 285 |
| 6 | KONA | Cultivated Crops | | None | | | |
| 6 | KONZ | Grassland Herbaceous | | None | | | |
| 6 | KUFS | Deciduous Forest | Random | Spring + Senescence | 75 | 210 | 330 |
| 7 | GRSM | Deciduous Forest | Random | Spring + Senescence | 90 | 215 | 310 |
| 7 | MLBS | Deciduous Forest | Random | Spring + Senescence | 110 | 220 | 310 |
| 7 | ORNL | Deciduous Forest | Random | Spring + Senescence | 90 | 210 | 315 |
| 8 | CHOC | Woody Wetlands | Targeted | Spring + Senescence | 70 | 200 | 335 |
| 8 | DELA | Woody Wetlands | Targeted | Spring + Senescence | 60 | 205 | 330 |
| 8 | TALL | Evergreen Forest | Random | Monthly, Year Round | 75 | 195 | 330 |
| 9 | DCFS | Grassland Herbaceous | | None | | | |
| 9 | NOGP | Grassland Herbaceous | | None | | | |
| 9 | WOOD | Grassland Herbaceous | | None | | | |
| 10 | CPER | Grassland Herbaceous | | None | | | |
| 10 | RMNP | Evergreen Forest | Random | Monthly, Year Round | 120 | 210 | 315 |
| 10 | STER | Cultivated Crops | | None | | | |
| 11 | CLBJ | Grassland Herbaceous | | None | | | |
| 11 | KLEM | #N/A | | | | | |
| 11 | TBD | #N/A | | | | | |
| 12 | BOZE | Grassland Herbaceous | | None | | | |
| 12 | PARA | Grassland Herbaceous | | None | | | |

| | | |
|------------------------------|------------------|----------------------|
| Title: | Author: K. Jones | Date: [Publish Date] |
| NEON Doc. #: NEON.DOC.001710 | | Revision: * |

| Domain | Site code | primary airshed NLCD | Trap Location Selection | Suggested Sampling Schedule | Average Greenness Increase | Beginning of Senescence | Average End of Senescence |
|--------|-----------|----------------------|-------------------------|-----------------------------|----------------------------|-------------------------|---------------------------|
| 12 | YELL | Shrub Scrub | TBD | TBD | 120 | 190 | 280 |
| 13 | MOAB | Shrub Scrub | TBD | TBD | 85 | 225 | 300 |
| 13 | NIWO | Grassland Herbaceous | | None | | | |
| 13 | TBD | #N/A | | | | | |
| 14 | JORN | Shrub Scrub | TBD | TBD | 80 | 245 | 320 |
| 14 | SRER | Shrub Scrub | TBD | None | 150 | 240 | 330 |
| 14 | TBD | #N/A | | | | | |
| 15 | ONAQ | Shrub Scrub | TBD | TBD | 75 | 170 | 280 |
| 15 | TBD | #N/A | | | | | |
| 15 | RBUT | Deciduous Forest | Random | Spring + Senescence | 105 | 190 | 310 |
| 16 | ABBY | Grassland Herbaceous | | None | | | |
| 16 | THAY | Evergreen Forest | Random | Monthly, Year Round | | | |
| 16 | WREF | Evergreen Forest | Random | Monthly, Year Round | | | |
| 17 | SJER | #N/A | Targeted | Monthly, Year Round | 270 | 95 | 155 |
| 17 | SOAP | Evergreen Forest | Random | Monthly, Year Round | 90 | 185 | 290 |
| 17 | TEAK | Evergreen Forest | Random | Monthly, Year Round | 120 | 205 | 300 |
| 18 | BARO | Sedge Herbaceous | | None | | | |
| 18 | TOOL | Dwarf Scrub | | TBD | 160 | 205 | 240 |
| 19 | BONA | Deciduous Forest | Random | Spring + Senescence | 135 | TBD | 250 |
| 19 | DEJU | Evergreen Forest | Random | Monthly, Year Round | | | |
| 19 | HEAL | Shrub Scrub | TBD | TBD | 135 | 210 | 245 |
| 19 | POKE | Deciduous Forest | Random | Spring + Senescence | 135 | 205 | 250 |
| 20 | OLAA | Evergreen Forest | Random | Monthly, Year Round | | | |
| 20 | PUFO | Shrub Scrub | Random | TBD | 0 | NA | 365 |
| 20 | PUGR | Grassland | | None | | | |

| | | |
|-------------------------------------|-------------------------|-----------------------------|
| <i>Title:</i> | <i>Author:</i> K. Jones | <i>Date:</i> [Publish Date] |
| <i>NEON Doc. #:</i> NEON.DOC.001710 | | <i>Revision:</i> * |

| Domain | Site code | primary airshed NLCD | Trap Location Selection | Suggested Sampling Schedule | Average Greenness Increase | Beginning of Senescence | Average End of Senescence |
|---------------|------------------|-----------------------------|--------------------------------|------------------------------------|-----------------------------------|--------------------------------|----------------------------------|
| | | Herbaceous | | | | | |

* Site information has been updated from NLCD or MODIS data based on local observations

| | | |
|------------------------------|------------------|----------------------|
| Title: | Author: K. Jones | Date: [Publish Date] |
| NEON Doc. #: NEON.DOC.001710 | | Revision: * |

APPENDIX E USING AND CALIBRATING THE TRUPULSE 360R LASER RANGEFINDER

Setting the Declination Offset

- 1) Press the “Power/Fire” button to turn on the unit. The viewfinder will display the main “Measurement Mode” screen.
- 2) Press and hold ▼ for 4 s to enter “System Setup Mode”.
- 3) Press ▼ until **H_Ang** is displayed in the viewfinder, then press “Power/Fire”.
- 4) **dECLn** will be displayed in the viewfinder, press “Power/Fire”.
- 5) **no** and **dECLn** will blink. Press ▼ until **YES** and **dECLn** blink, then press “Power/Fire” again. The current declination is shown in the viewfinder.
- 6) If this is the correct value, press and hold ▲ to return to the main “Measurement Mode” screen.
- 7) If the displayed value is incorrect for your current location:
 - a) Press either ▲ or ▼ to change the tenths value, press “Power/fire”.
 - b) Press either ▲ or ▼ to change first integer value, press “Power/fire”.
 - c) Press either ▲ or ▼ to change second integer value, press “Power/fire”.
 - d) The value just entered will blink. Press “Power/fire” to confirm and return to the “Measurement Mode” screen.

Tilt Sensor Calibration

- 1) Press the “Power/Fire” button to turn on the unit. The viewfinder will display the main “Measurement Mode” screen.
- 2) Press and Press and hold ▼ for 4 s to enter “System Setup Mode”.
- 3) Press ▼ until **inC** is displayed in the viewfinder, then press “Power/Fire”..
- 4) **no** and **CAL** will blink. Press ▼ until **yes** and **CAL** blink, then press “Power/Fire” again.
 - a) Calibration can be aborted by pressing “Power/Fire” when **no** and **CAL** are alternately displayed.
- 5) **C1_Fd** will be displayed in the view finder.
- 6) Place the TruPulse on a flat, relatively flat surface (within 15deg of level). Follow the sequence outlined in Figure 4.
 - a) At each step wait approximately 1 second before pressing “Power/fire”, then wait another second before moving to the next position. It is important that the unit is held steady when you press “Power/fire”.
 - b) To abort and return to previous calibration at any point hold ▲ or ▼ for 4 sec.

| | | |
|------------------------------|------------------|----------------------|
| Title: | Author: K. Jones | Date: [Publish Date] |
| NEON Doc. #: NEON.DOC.001710 | | Revision: * |

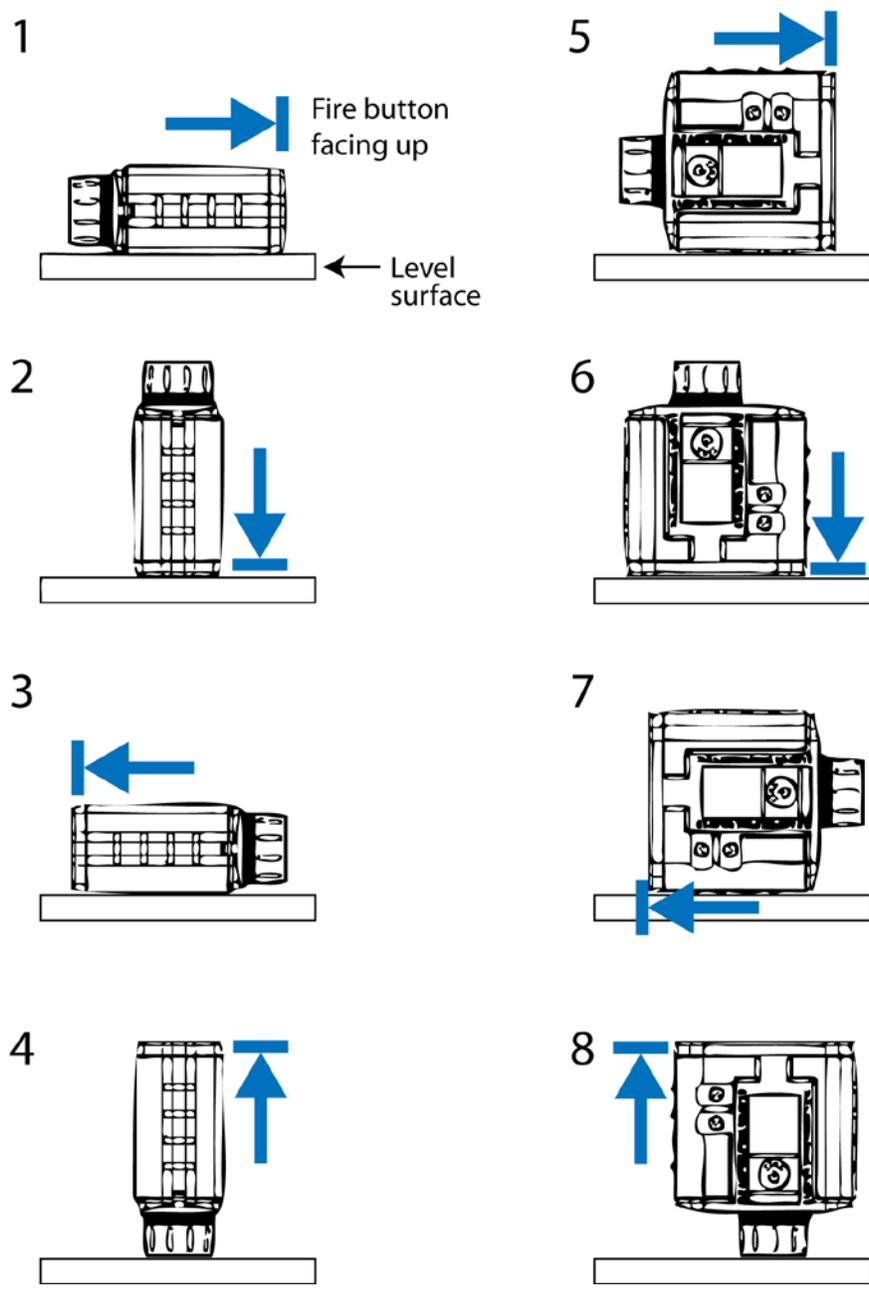


Figure 5. The tilt-sensor calibration routine for the TruPulse 360R laser rangefinder. The blue arrow and line indicate the direction of the lens at each calibration step.

| | | |
|------------------------------|------------------|----------------------|
| Title: | Author: K. Jones | Date: [Publish Date] |
| NEON Doc. #: NEON.DOC.001710 | | Revision: * |

- 7) After all 8 positions have been run through, look through the eyepiece. Either a **PASS** or **FAiL** message appears in the view finder.
 - a) **PASS**: Press the “Power/Fire” Button to return to the measurement mode.
 - b) **FAiL1**: Excessive motion during calibration. Unit was not held steady.
 - c) **FAiL2**: Magnetic saturation error. Local magnetic field too strong.
 - d) **FAiL3**: Mathematical fit error.
 - e) **FAiL4**: Calibration convergence error.
 - f) **FAiL6**: Orientations were wrong during the calibrations.
- 8) If **FAiL** appears, press the “Power/Fire” button. **No** and **CAL** will alternately blink allowing you to do a new calibration. IF the calibration fails, the unit reverts to the previous calibration.

Using and Calibrating the TruPulse 360R Compass

Like any compass, the internal compass of the TruPulse is susceptible to error and to interference from common metallic objects. The following objects may affect the compass performance, and should be kept at least 50 cm (20 in) away from the TruPulse during operation:

| | |
|------------------------------|---------------------------|
| Batteries | Nails |
| Data collectors or computers | Pin flags w/ metal stakes |
| Portable electronics | Steel-rimmed eyeglasses |
| Metal watch bands | Eyeglass spring-hinges |
| Non-aluminum tripods | |

When using the TruPulse compass, it is good practice to check the compass performance against a standard mirror-site compass or a previously established plot-line at the beginning of each day, or when beginning a new plot. In addition, ALWAYS CHECK AND RECALIBRATE THE COMPASS AFTER CHANGING THE BATTERIES. It is common for the compass calibration to be inaccurate when the low battery indicator is displayed in the viewfinder, and you should always replace the batteries when this indicator appears.

If the compass requires calibrating, you must first determine that you are in an area free from local magnetic interference. Either of the following simple tests can be used in the field to test for local magnetic interference:

- 1) Choose a target at least 100 m away, and shoot to it. Note the azimuth. Then step backward or forward 1 m along the sight-line to the target and shoot again. Note the second azimuth.
 - The second azimuth should be within 1/10 to 5/10 of a degree of the first azimuth. If it is, you are likely in an anomaly-free area.
 - For increased confidence, repeat the test with a second target at 90° to the azimuth of the first target.
- 2) Select a target at least 10 m away, shoot to it, and note the azimuth. Move to the target that was just shot, and shoot back toward the spot that was just occupied. Note the second azimuth.

| | | |
|------------------------------|------------------|----------------------|
| Title: | Author: K. Jones | Date: [Publish Date] |
| NEON Doc. #: NEON.DOC.001710 | | Revision: * |

- The two azimuths should be 180° different, plus or minus no more than a few tenths of a degree.

Once you have ascertained that the current location is free from local magnetic interference, complete the following steps to calibrate the TruPulse 360R compass:

- 1) Press the “Power/Fire” button to turn on the unit. The viewfinder will display the main “Measurement Mode” screen.
- 2) Press and hold ▼ for 4 s to enter “System Setup Mode”.
- 3) Press ▼ until **H_Ang** is displayed in the viewfinder, then press “Power/Fire”..
- 4) **dECLn** is displayed. Press ▼ to display the **HACAL** option, then press “Power/Fire” again.
- 5) **No** and **HACAL** will alternately blink. Press ▲ or ▼ to display **YES** and **CAL**, then press “Power/Fire” to begin calibration.
 - Calibration can be aborted by pressing “Power/Fire” when **no** and **CAL** are alternately displayed.
- 6) **C1_Fd** will be displayed in the view finder.
- 7) Use a standard mirror-site compass to determine the direction of **magnetic** North. Holding the TruPulse 360R and facing close to **magnetic** North ($\pm 15^\circ$), the lenses should be facing as shown in Figure 5. To complete the calibration routine, follow the sequence outlined in Figure 5.
 - At each step wait approximately 1 second before pressing “Power/fire”, then wait another second before moving to the next position. It is important that the unit is held steady when you press “Power/fire”.
 - To abort and return to previous calibration at any point hold ▲ or ▼ for 4 sec.
- 8) After all 8 positions have been run through in sequence, look through the eyepiece. Either a **PASS** or **FAiL** message appears in the view finder.
 - **PASS**: Press the “Power/Fire” Button to return to the measurement mode.
 - **FAiL1**: Excessive motion during calibration. Unit was not held steady.
 - **FAiL2**: Magnetic saturation error. Local magnetic field too strong.
 - **FAiL3**: Mathematical fit error.
 - **FAiL4**: Calibration convergence error.
 - **FAiL6**: Orientations were wrong during the calibrations.

If **FAiL** appears, press the “Power/Fire” button. **No** and **CAL** will alternately blink allowing you to do a new calibration. If the calibration fails, the unit reverts to the previous calibration.

| | | |
|------------------------------|------------------|----------------------|
| Title: | Author: K. Jones | Date: [Publish Date] |
| NEON Doc. #: NEON.DOC.001710 | | Revision: * |

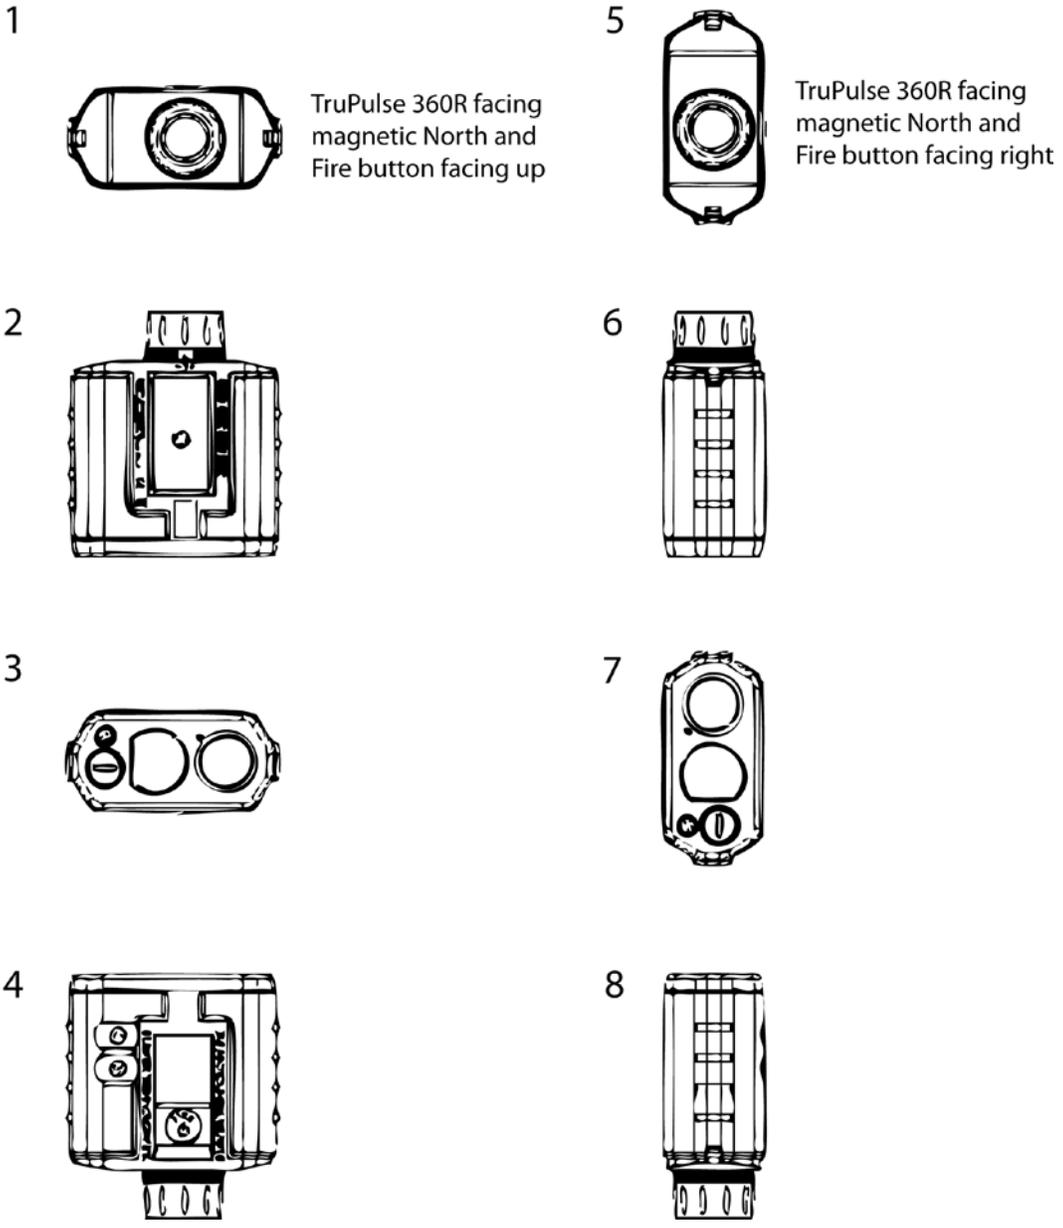


Figure 6. The internal compass calibration routine for the TruPulse 360R laser rangefinder.

| | | |
|------------------------------|------------------|----------------------|
| Title: | Author: K. Jones | Date: [Publish Date] |
| NEON Doc. #: NEON.DOC.001710 | | Revision: * |

Measuring Distance from a Known Point

- 1) Press “Power/Fire” to turn on the TruPulse.
- 2) Set the unit to Target Mode = Filter
 - a) Press ▲ for 4 seconds. The active Target Mode appears in the viewfinder. Press ▲ or ▼ to cycle through available Target Modes.
Available Target Modes are:

Table 11. Laser Target Modes available for the TruPulse 360 laser rangefinder/clinometer models.

| Target Mode | Definition | When to Use |
|-------------|--|--|
| Std | Standard, single-shot | Clear shot to unobstructed target |
| Con | Continuous; pressing and holding “Power /Fire” will continuously acquire targets for up to 10 s | Useful for scanning trees in order to find the highest point |
| CLO | Closest; pressing and holding “Power /Fire” will acquire multiple targets, the viewfinder displays the closest target | Narrow targets in the foreground |
| FAR | Farthest; identical to CLO, but the viewfinder displays the farthest target | <ul style="list-style-type: none"> • Target partially obscured by brush • Finding highest point of a tree |
| Flt | Filter; the sensor sensitivity is reduced to only detect laser pulses returned from a reflective surface; <i>F’ appears in the viewfinder</i> | <ul style="list-style-type: none"> • Measuring targets through thick brush • In very heavy brush, the optional foliage filter can be used in this mode (but is not required) |

- b) Choose “Flt” and press “Power/Fire” to make the chosen Target Mode active.
- 3) Press either the ▲ or ▼ button until **HD** (i.e. Horizontal Distance) appears in the viewfinder.
- 4) Person 1: Hold the reflective surface at the base of the stem so that it is visible to Person 2.
- 5) Person 2: Look through the TruPulse viewfinder, aim the crosshairs at the reflective surface held by Person 1, and press and hold “Power/Fire” until the distance is displayed in the viewfinder; record this distance.

Measuring Azimuth from a Known Point

- 1) After recording the **HD** to the stem above, press ▲ three times until **AZ** (i.e. azimuth from True North) appears in the viewfinder and the angle in degrees is displayed; record this angle.

The angle should be preceded by a “d” indicating that declination has been set for the TruPulse at your current location (as described previously).