

<i>Title:</i> NEON Algorithm Theoretical Basis Document (ATBD): Surface Water Nitrate		<i>Date:</i> 12/04/2018
<i>NEON Doc. #:</i> NEON.DOC.002181	<i>Author:</i> J. Vance	<i>Revision:</i> B

ALGORITHM THEORETICAL BASIS DOCUMENT (ATBD):

SURFACE WATER NITRATE

PREPARED BY	ORGANIZATION	DATE
Jesse Vance	AQU	12/04/2018
Kaelin M Cawley	AQU	09/03/2018
Derek Smith	FIU	01/06/2014
Josh Roberti	FIU	01/15/2014

APPROVALS	ORGANIZATION	APPROVAL DATE
Kate Thibault	SCI	01/03/2019
Mike Stewart	PSE	01/02/2019

RELEASED BY	ORGANIZATION	RELEASE DATE
Anne Balsley	CM	01/03/2018

See configuration management system for approval history.

The National Ecological Observatory Network is a project solely funded by the National Science Foundation and managed under cooperative agreement by Battelle. Any opinions, findings, and conclusions or recommendations expressed in this material are those of the author(s) and do not necessarily reflect the views of the National Science Foundation.

<i>Title:</i> NEON Algorithm Theoretical Basis Document (ATBD): Surface Water Nitrate		<i>Date:</i> 12/04/2018
<i>NEON Doc. #:</i> NEON.DOC.002181	<i>Author:</i> J. Vance	<i>Revision:</i> B

Change Record

REVISION	DATE	ECO #	DESCRIPTION OF CHANGE
A	09/12/2017	ECO-04874	Initial Release
B	01/03/2019	ECO-05951	Revised averaging window per configuration change

Title: NEON Algorithm Theoretical Basis Document (ATBD): Surface Water Nitrate		Date: 12/04/2018
NEON Doc. #: NEON.DOC.002181	Author: J. Vance	Revision: B

TABLE OF CONTENTS

1 DESCRIPTION.....2

1.1 Purpose 2

1.2 Scope..... 3

2 RELATED DOCUMENTS, ACRONYMS AND VARIABLE NOMENCLATURE4

2.1 Applicable Documents 4

2.2 Reference Documents..... 4

2.3 Acronyms 4

2.4 Variable Nomenclature 5

3 DATA PRODUCT DESCRIPTION.....6

3.1 Variables Reported 6

3.2 Input Dependencies 6

3.3 Product Instances..... 6

3.4 Temporal Resolution and Extent 6

3.5 Spatial Resolution and Extent 6

4 SCIENTIFIC CONTEXT7

4.1 Theory of Measurement 8

4.2 Theory of Algorithm 9

5 ALGORITHM IMPLEMENTATION.....18

6 UNCERTAINTY21

6.1 Uncertainty of Surface Water Nitrate..... 21

6.1.1 Measurement Uncertainty..... 22

6.1.2 Uncertainty of the L1 Mean Data Products 24

6.2 Expanded Uncertainty..... 26

6.1 Uncertainty Budget..... 26

7 FUTURE PLANS AND MODIFICATIONS.....27

8 BIBLIOGRAPHY27

<i>Title:</i> NEON Algorithm Theoretical Basis Document (ATBD): Surface Water Nitrate		<i>Date:</i> 12/04/2018
<i>NEON Doc. #:</i> NEON.DOC.002181	<i>Author:</i> J. Vance	<i>Revision:</i> B

LIST OF TABLES AND FIGURES

Table 3-1: List of Surface Water Nitrate-related L0 DPs that are transformed into L1 Surface Water Nitrate DPs in this ATBD..... 6

Table 2. Data fields and position that are captured with the SUNA and placed into the concatenated string, L0 data stream, identified in Table 3-1 above. 9

Table 5-1: Flags associated with Surface Water Nitrate measurements..... 20

Table 5-2: Information maintained in the CI data store for Surface Water Nitrate. 21

Table 5. Uncertainty budget for individual measurements. Shaded rows denote the order of uncertainty propagation (from lightest to darkest). 26

Table 6. Uncertainty budget for L1 mean DPs. Shaded rows denote the order of uncertainty propagation (from lightest to darkest)..... 27

Figure 1. Schematic of nitrogen cycle in aquatic environmetns..... 8

Figure 2. Absorbance spectra for bromide, nitrate, hydrogen sulfide and nitrite in the ultraviolet range. 9

Figure 3. Displays the data flow and associated uncertainties of individual measurements of surface water nitrate and associated L1 DPs..... 22

1 DESCRIPTION

Contained in this document are details concerning temperature measurements made at all NEON sites. Specifically, the processes necessary to convert “raw” sensor measurements into meaningful scientific units and their associated uncertainties are described. Nitrate will be continuously monitored at all core and relocatable sites via a submersible ultraviolet nitrate analyzer.

1.1 Purpose

This document details the algorithms used for creating NEON Level 1 data products for Surface Water Nitrate from Level 0 data, and ancillary data as defined in this document (such as calibration data) obtained via instrumental measurements made by the Nitrate Analyzer. It includes a detailed discussion of measurement theory and implementation, appropriate theoretical background, data product provenance, quality assurance and control methods used, approximations and/or assumptions made, and a detailed exposition of uncertainty resulting in a cumulative reported uncertainty for this product.

<i>Title:</i> NEON Algorithm Theoretical Basis Document (ATBD): Surface Water Nitrate		<i>Date:</i> 12/04/2018
<i>NEON Doc. #:</i> NEON.DOC.002181	<i>Author:</i> J. Vance	<i>Revision:</i> B

1.2 Scope

The theoretical background and entire algorithmic process used to derive Level 1 data from Level 0 data for Surface Water Nitrate is described in this document. The Nitrate Analyzer employed is the SUNA V2 Submersible Ultraviolet Nitrate Analyzer manufactured by Satlantic LP. This document does not provide computational implementation details, except for cases where these stem directly from algorithmic choices explained here.

Title: NEON Algorithm Theoretical Basis Document (ATBD): Surface Water Nitrate		Date: 12/04/2018
NEON Doc. #: NEON.DOC.002181	Author: J. Vance	Revision: B

2 RELATED DOCUMENTS, ACRONYMS AND VARIABLE NOMENCLATURE

2.1 Applicable Documents

AD[01]	NEON.DOC.000001	NEON OBSERVATORY DESIGN
AD[02]	NEON.DOC.005003	NEON Scientific Data Products Catalog
AD[03]	NEON.DOC.002652	NEON Level 1, Level 2 and Level 3 Data Products Catalog
AD[04]	NEON.DOC.005005	NEON Level 0 Data Products Catalog
AD[05]	NEON.DOC.000782	ATBD QA/QC Data Consistency
AD[06]	NEON.DOC.011081	ATBD QA/QC Plausibility Tests
AD[07]	NEON.DOC.000783	ATBD De-spiking and Time Series Analyses
AD[08]	NEON.DOC.000746	Calibration Fixture and Sensor Uncertainty Analysis (CVAL)
AD[09]	NEON.DOC.000785	TIS Level 1 Data Products Uncertainty Budget Estimation Plan
AD[10]	NEON.DOC.000927	NEON Calibration and Sensor Uncertainty Values ¹
AD[11]	NEON.DOC.001113	Quality Flags and Quality Metrics for TIS Data Products
AD[13]	NEON.DOC.001570	NEON Sensor Command, Control and Configuration Document: SUNA Nitrate Analyzer, Wadeable Streams
AD[14]	NEON.DOC.000597	STCDD – 0329950000 – Sensor, Suna Nutrient with Integrated Wiper
AD[15]	NEON.DOC.003808	NEON Sensor Command, Control and Configuration Document: Buoy Meteorological Station and Submerged Sensor Assembly
AD[16]	NEON.DOC.003824	STCDD – 0329950100 – Sensor, Buoy, SUNA Nitrate with Integrated Wiper, Titanium Housing

¹ Note that CI obtains calibration and sensor values directly from an XML file maintained and updated by CVAL in real time. This report is updated approximately quarterly such that there may be a lag time between the XML and report updates.

2.2 Reference Documents

RD[01]	NEON.DOC.000008	NEON Acronym List
RD[02]	NEON.DOC.000243	NEON Glossary of Terms

2.3 Acronyms

Acronym	Explanation
AIS	Aquatic Instrument System
ATBD	Algorithm Theoretical Basis Document
CI	NEON Cyberinfrastructure
CVAL	NEON Calibration, Validation, and Audit Laboratory
DAS	Data Acquisition System

Title: NEON Algorithm Theoretical Basis Document (ATBD): Surface Water Nitrate		Date: 12/04/2018
NEON Doc. #: NEON.DOC.002181	Author: J. Vance	Revision: B

DP	Data Product
FDAS	Field Data Acquisition System
GRAPE	Grouped Remote Analog Peripheral Equipment
Hz	Hertz
L0	Level 0
L1	Level 1
PRT	Platinum resistance thermometer
QA/QC	Quality assurance and quality control

2.4 Variable Nomenclature

The symbols used to display the various inputs in the ATBD, e.g., calibration coefficients and uncertainty estimates, were chosen so that the equations can be easily interpreted by the reader. However, the symbols provided will not always reflect NEON’s internal notation, which is relevant for CI’s use, and/or the notation that is used to present variables on NEON’s data portal. Therefore a lookup table is provided in order to distinguish what symbols specific variables can be tied to in the following document.

Symbol	Internal Notation	Description
u_{A1}	U_CVALA1	Combined, standard uncertainty of the SUNA nitrate sensor (μM)
u_{A3}	U_CVALA3	Combined, relative uncertainty of the SUNA nitrate sensor (%)
H	Parse from L0 string (field 271)	Internal humidity of sensor
$SpAv_L$	Parse from L0 string (field 8)	Spectrum average during light frame
$SpAv_D$	Parse from L0 string (field 9)	Spectrum average during dark frame
NO_3	Parse from L0 string (field 3)	Nitrate Value in micromoles per liter (μM)

Title: NEON Algorithm Theoretical Basis Document (ATBD): Surface Water Nitrate		Date: 12/04/2018
NEON Doc. #: NEON.DOC.002181	Author: J. Vance	Revision: B

3 DATA PRODUCT DESCRIPTION

3.1 Variables Reported

The Surface Water Nitrate-related L1 DPs provided by the algorithms documented in this ATBD are displayed in the accompanying file: `swn_datapub_NEONDOC004046.txt`.

3.2 Input Dependencies

Table 1 details the Surface Water Nitrate-related L0 DPs used to produce L1 Surface Water Nitrate DPs in this ATBD.

Table 3-1: List of Surface Water Nitrate-related L0 DPs that are transformed into L1 Surface Water Nitrate DPs in this ATBD.

Description	Sample Frequency	Units	Data Product Number
Nitrate in surface water	burst of 1 dark frame and 20 light frames	NA	NEON.DOM.SITE.DP0.20033.001.02242.HOR.VER.000

3.3 Product Instances

One Nitrate Analyzer will be deployed at each AQU site. At wadeable stream sites the SUNA will be installed in the stream channel at the S2 location and will be mounted onto the in-stream infrastructure that is shared with other submerged aquatic sensors (multisonde, prt and LevelTroll). At lake and river sites, the SUNA will be deployed off of the buoy approximately 1.5m below the surface.

3.4 Temporal Resolution and Extent

L0 data will be collected in burst measurements every 15 minutes, where each burst consists of 1 dark frame and 20 light frames. A portion of the sampling window is averaged and treated as a single instantaneous point measurement every 15 minutes to form L1 DPs.

3.5 Spatial Resolution and Extent

The spatial resolution and extent represented by the SUNA will vary depending on the aquatic feature the sensor is placed in. In streams the SUNA will be located at only S2 and deployed at a fixed depth. This position will be chosen to represent the bulk water mass in the stream. In rivers and lakes the SUNA will be located at a fixed depth to monitor relative changes; however extrapolation to the broader aquatic system will require additional observational measurements.

<i>Title:</i> NEON Algorithm Theoretical Basis Document (ATBD): Surface Water Nitrate		<i>Date:</i> 12/04/2018
<i>NEON Doc. #:</i> NEON.DOC.002181	<i>Author:</i> J. Vance	<i>Revision:</i> B

4 SCIENTIFIC CONTEXT

Nitrate is a form of nitrogen, one of the primary nutrients (carbon, nitrogen, and phosphorous) in aquatic and terrestrial ecosystems. It is formed during the breakdown of organic material, the production of nitrogen fixing-plants, and industrial production. Figure 1 illustrates how nitrate is formed and utilized in aquatic environments relative to other forms of nitrogen. While nitrate is often the limiting nutrient for photosynthesis in marine environments it is not the limiting nutrient in freshwater. Human activities and various land-uses such as agriculture, urban and industrial areas can lead to excess nitrate in surface and ground waters.

Levels of nutrients in the environment indicate the health of the ecosystem. Excess nutrients in the system stimulate rapid primary production (growth by plants and algae), which can include blooms of toxic algae. As the plants and algae die they are decomposed by microbes in the water which consume oxygen. This reduction in dissolved oxygen can be harmful to fish and other aquatic organism and lower the overall health of the ecosystem.

Measuring nitrate in aquatic systems is critical to understanding the biogeochemical cycle and mechanisms in the ecosystem. Changes in the concentration of nitrate over time may be an indication of shifts in the trophic structure and community composition of the aquatic ecosystem.

Aquatic Nitrogen Cycle

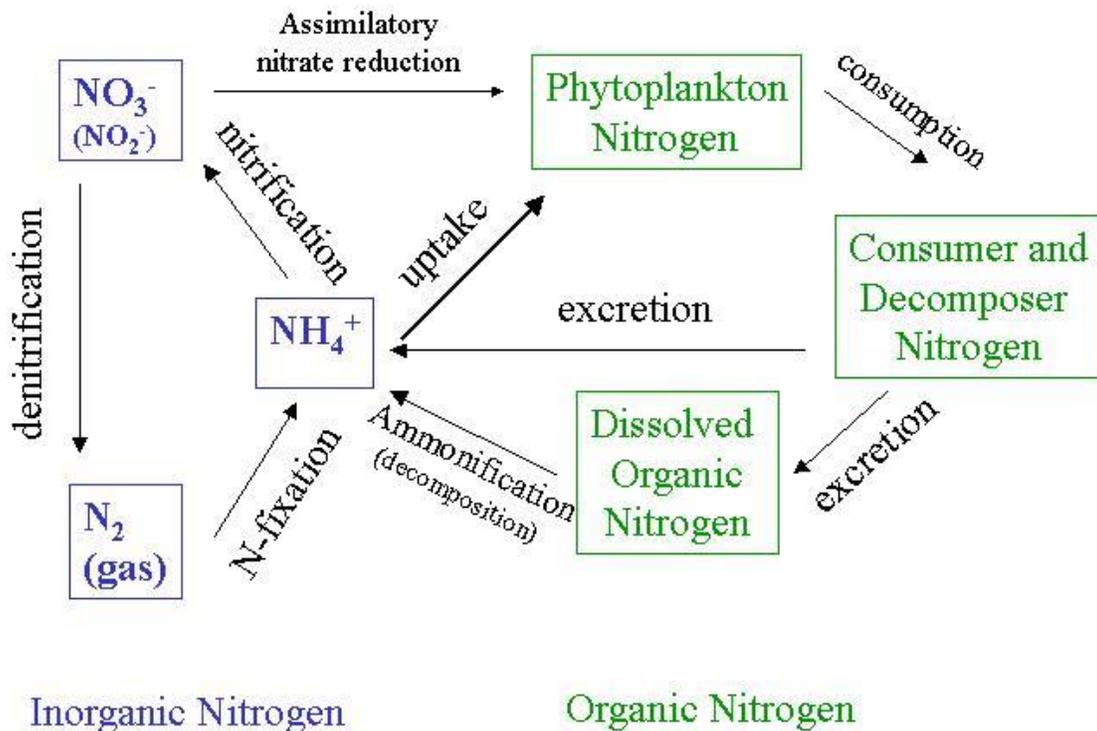


Figure 1. Schematic of nitrogen cycle in aquatic environments.

4.1 Theory of Measurement

Nitrate is one of several inorganic chemical species that strongly absorb ultraviolet light (wavelength <280nm). Other species of importance include bromide and hydrogen sulfide and some organic compounds (see Figure 2). Measuring nitrate in aquatic systems can be difficult because of the overlapping absorbance bands of different chemical species.

The principle of the measurement consists of applying a UV light source across the water sample; the nitrate (and other species) absorb energy from the light in the state of its electrons; a spectrometer then measures how much light passed through the sample at each wavelength. The absorbance signal due to nitrate in the water is proportional to its concentration in the sample. It is critical to have a stable light source and a spectrometer capable of resolving the spectra for the nitrate in the water.

The SUNA consists of a high-resolution spectrometer that is optimized for UV range wavelengths, a stable deuterium lamp, an on-board controller and a data storage device. The SUNA internally converts all signals to digital data and applies algorithms developed by MBARI and Satlantic specific to this instrument prior to output.

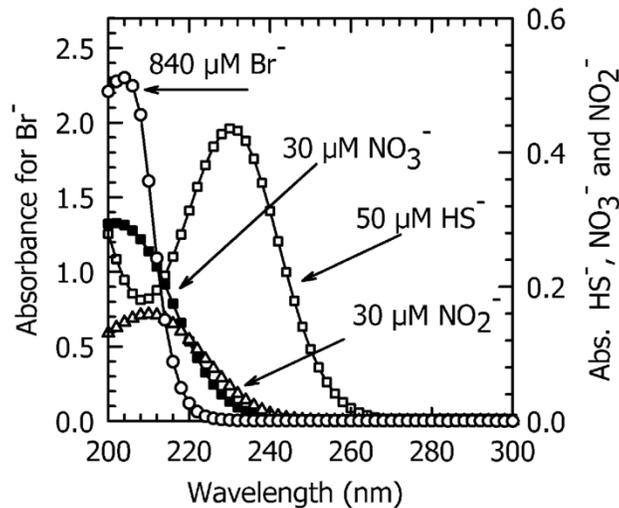


Figure 2. Absorbance spectra for bromide, nitrate, hydrogen sulfide and nitrite in the ultraviolet range.

4.2 Theory of Algorithm

The SUNA nitrate sensor produces an ASCII file that contains 285 data fields. To accommodate this large number of fields, the data fields are concatenated such that each measurement is reported as a single string of characters, where the fields are identified by the numeric field ID followed by a colon and the measurement value. Each field is delimited by commas. This data transmission scheme is illustrated in Equation 1.

$$\text{Measurement string\#0} = \{0: \langle \text{value} \rangle, 1: \langle \text{value} \rangle, \dots, 285: \langle \text{value} \rangle\} \tag{Equation 1}$$

Where each field has a numerical index followed by the measurement value.

The identification of the data fields is given in Table 2.

Table 2. Data fields and position that are captured with the SUNA and placed into the concatenated string, L0 data stream, identified in Table 3-1 above.

L0 Data Stream Field Position	Full ASCII Data Fields
0	Light Frame/Dark Frame
1	Date field (numeric)
2	Time field (numeric)
3	Nitrate concentration as micromolar
4	Nitrogen in nitrate as mg/L
5	Absorbance at 254 nm
6	Absorbance at 350 nm

Title: NEON Algorithm Theoretical Basis Document (ATBD): Surface Water Nitrate		Date: 12/04/2018
NEON Doc. #: NEON.DOC.002181	Author: J. Vance	Revision: B

7	Bromide trace
8	Spec Average or SW Average(Dark Correction Method)
9	Dark Signal Average (average dark intensity)
10	Integration Time Factor
11	spectrometer intensity at wavelength #1
12	spectrometer intensity at wavelength #2
13	spectrometer intensity at wavelength #3
14	spectrometer intensity at wavelength #4
15	spectrometer intensity at wavelength #5
16	spectrometer intensity at wavelength #6
17	spectrometer intensity at wavelength #7
18	spectrometer intensity at wavelength #8
19	spectrometer intensity at wavelength #9
20	spectrometer intensity at wavelength #10
21	spectrometer intensity at wavelength #11
22	spectrometer intensity at wavelength #12
23	spectrometer intensity at wavelength #13
24	spectrometer intensity at wavelength #14
25	spectrometer intensity at wavelength #15
26	spectrometer intensity at wavelength #16
27	spectrometer intensity at wavelength #17
28	spectrometer intensity at wavelength #18
29	spectrometer intensity at wavelength #19
30	spectrometer intensity at wavelength #20
31	spectrometer intensity at wavelength #21
32	spectrometer intensity at wavelength #22
33	spectrometer intensity at wavelength #23
34	spectrometer intensity at wavelength #24
35	spectrometer intensity at wavelength #25
36	spectrometer intensity at wavelength #26
37	spectrometer intensity at wavelength #27
38	spectrometer intensity at wavelength #28
39	spectrometer intensity at wavelength #29
40	spectrometer intensity at wavelength #30
41	spectrometer intensity at wavelength #31
42	spectrometer intensity at wavelength #32
43	spectrometer intensity at wavelength #33

Title: NEON Algorithm Theoretical Basis Document (ATBD): Surface Water Nitrate		Date: 12/04/2018
NEON Doc. #: NEON.DOC.002181	Author: J. Vance	Revision: B

44	spectrometer intensity at wavelength #34
45	spectrometer intensity at wavelength #35
46	spectrometer intensity at wavelength #36
47	spectrometer intensity at wavelength #37
48	spectrometer intensity at wavelength #38
49	spectrometer intensity at wavelength #39
50	spectrometer intensity at wavelength #40
51	spectrometer intensity at wavelength #41
52	spectrometer intensity at wavelength #42
53	spectrometer intensity at wavelength #43
54	spectrometer intensity at wavelength #44
55	spectrometer intensity at wavelength #45
56	spectrometer intensity at wavelength #46
57	spectrometer intensity at wavelength #47
58	spectrometer intensity at wavelength #48
59	spectrometer intensity at wavelength #49
60	spectrometer intensity at wavelength #50
61	spectrometer intensity at wavelength #51
62	spectrometer intensity at wavelength #52
63	spectrometer intensity at wavelength #53
64	spectrometer intensity at wavelength #54
65	spectrometer intensity at wavelength #55
66	spectrometer intensity at wavelength #56
67	spectrometer intensity at wavelength #57
68	spectrometer intensity at wavelength #58
69	spectrometer intensity at wavelength #59
70	spectrometer intensity at wavelength #60
71	spectrometer intensity at wavelength #61
72	spectrometer intensity at wavelength #62
73	spectrometer intensity at wavelength #63
74	spectrometer intensity at wavelength #64
75	spectrometer intensity at wavelength #65
76	spectrometer intensity at wavelength #66
77	spectrometer intensity at wavelength #67
78	spectrometer intensity at wavelength #68
79	spectrometer intensity at wavelength #69
80	spectrometer intensity at wavelength #70
81	spectrometer intensity at wavelength #71

Title: NEON Algorithm Theoretical Basis Document (ATBD): Surface Water Nitrate		Date: 12/04/2018
NEON Doc. #: NEON.DOC.002181	Author: J. Vance	Revision: B

82	spectrometer intensity at wavelength #72
83	spectrometer intensity at wavelength #73
84	spectrometer intensity at wavelength #74
85	spectrometer intensity at wavelength #75
86	spectrometer intensity at wavelength #76
87	spectrometer intensity at wavelength #77
88	spectrometer intensity at wavelength #78
89	spectrometer intensity at wavelength #79
90	spectrometer intensity at wavelength #80
91	spectrometer intensity at wavelength #81
92	spectrometer intensity at wavelength #82
93	spectrometer intensity at wavelength #83
94	spectrometer intensity at wavelength #84
95	spectrometer intensity at wavelength #85
96	spectrometer intensity at wavelength #86
97	spectrometer intensity at wavelength #87
98	spectrometer intensity at wavelength #88
99	spectrometer intensity at wavelength #89
100	spectrometer intensity at wavelength #90
101	spectrometer intensity at wavelength #91
102	spectrometer intensity at wavelength #92
103	spectrometer intensity at wavelength #93
104	spectrometer intensity at wavelength #94
105	spectrometer intensity at wavelength #95
106	spectrometer intensity at wavelength #96
107	spectrometer intensity at wavelength #97
108	spectrometer intensity at wavelength #98
109	spectrometer intensity at wavelength #99
110	spectrometer intensity at wavelength #100
111	spectrometer intensity at wavelength #101
112	spectrometer intensity at wavelength #102
113	spectrometer intensity at wavelength #103
114	spectrometer intensity at wavelength #104
115	spectrometer intensity at wavelength #105
116	spectrometer intensity at wavelength #106
117	spectrometer intensity at wavelength #107
118	spectrometer intensity at wavelength #108
119	spectrometer intensity at wavelength #109

Title: NEON Algorithm Theoretical Basis Document (ATBD): Surface Water Nitrate		Date: 12/04/2018
NEON Doc. #: NEON.DOC.002181	Author: J. Vance	Revision: B

120	spectrometer intensity at wavelength #110
121	spectrometer intensity at wavelength #111
122	spectrometer intensity at wavelength #112
123	spectrometer intensity at wavelength #113
124	spectrometer intensity at wavelength #114
125	spectrometer intensity at wavelength #115
126	spectrometer intensity at wavelength #116
127	spectrometer intensity at wavelength #117
128	spectrometer intensity at wavelength #118
129	spectrometer intensity at wavelength #119
130	spectrometer intensity at wavelength #120
131	spectrometer intensity at wavelength #121
132	spectrometer intensity at wavelength #122
133	spectrometer intensity at wavelength #123
134	spectrometer intensity at wavelength #124
135	spectrometer intensity at wavelength #125
136	spectrometer intensity at wavelength #126
137	spectrometer intensity at wavelength #127
138	spectrometer intensity at wavelength #128
139	spectrometer intensity at wavelength #129
140	spectrometer intensity at wavelength #130
141	spectrometer intensity at wavelength #131
142	spectrometer intensity at wavelength #132
143	spectrometer intensity at wavelength #133
144	spectrometer intensity at wavelength #134
145	spectrometer intensity at wavelength #135
146	spectrometer intensity at wavelength #136
147	spectrometer intensity at wavelength #137
148	spectrometer intensity at wavelength #138
149	spectrometer intensity at wavelength #139
150	spectrometer intensity at wavelength #140
151	spectrometer intensity at wavelength #141
152	spectrometer intensity at wavelength #142
153	spectrometer intensity at wavelength #143
154	spectrometer intensity at wavelength #144
155	spectrometer intensity at wavelength #145
156	spectrometer intensity at wavelength #146
157	spectrometer intensity at wavelength #147

Title: NEON Algorithm Theoretical Basis Document (ATBD): Surface Water Nitrate		Date: 12/04/2018
NEON Doc. #: NEON.DOC.002181	Author: J. Vance	Revision: B

158	spectrometer intensity at wavelength #148
159	spectrometer intensity at wavelength #149
160	spectrometer intensity at wavelength #150
161	spectrometer intensity at wavelength #151
162	spectrometer intensity at wavelength #152
163	spectrometer intensity at wavelength #153
164	spectrometer intensity at wavelength #154
165	spectrometer intensity at wavelength #155
166	spectrometer intensity at wavelength #156
167	spectrometer intensity at wavelength #157
168	spectrometer intensity at wavelength #158
169	spectrometer intensity at wavelength #159
170	spectrometer intensity at wavelength #160
171	spectrometer intensity at wavelength #161
172	spectrometer intensity at wavelength #162
173	spectrometer intensity at wavelength #163
174	spectrometer intensity at wavelength #164
175	spectrometer intensity at wavelength #165
176	spectrometer intensity at wavelength #166
177	spectrometer intensity at wavelength #167
178	spectrometer intensity at wavelength #168
179	spectrometer intensity at wavelength #169
180	spectrometer intensity at wavelength #170
181	spectrometer intensity at wavelength #171
182	spectrometer intensity at wavelength #172
183	spectrometer intensity at wavelength #173
184	spectrometer intensity at wavelength #174
185	spectrometer intensity at wavelength #175
186	spectrometer intensity at wavelength #176
187	spectrometer intensity at wavelength #177
188	spectrometer intensity at wavelength #178
189	spectrometer intensity at wavelength #179
190	spectrometer intensity at wavelength #180
191	spectrometer intensity at wavelength #181
192	spectrometer intensity at wavelength #182
193	spectrometer intensity at wavelength #183
194	spectrometer intensity at wavelength #184
195	spectrometer intensity at wavelength #185

Title: NEON Algorithm Theoretical Basis Document (ATBD): Surface Water Nitrate		Date: 12/04/2018
NEON Doc. #: NEON.DOC.002181	Author: J. Vance	Revision: B

196	spectrometer intensity at wavelength #186
197	spectrometer intensity at wavelength #187
198	spectrometer intensity at wavelength #188
199	spectrometer intensity at wavelength #189
200	spectrometer intensity at wavelength #190
201	spectrometer intensity at wavelength #191
202	spectrometer intensity at wavelength #192
203	spectrometer intensity at wavelength #193
204	spectrometer intensity at wavelength #194
205	spectrometer intensity at wavelength #195
206	spectrometer intensity at wavelength #196
207	spectrometer intensity at wavelength #197
208	spectrometer intensity at wavelength #198
209	spectrometer intensity at wavelength #199
210	spectrometer intensity at wavelength #200
211	spectrometer intensity at wavelength #201
212	spectrometer intensity at wavelength #202
213	spectrometer intensity at wavelength #203
214	spectrometer intensity at wavelength #204
215	spectrometer intensity at wavelength #205
216	spectrometer intensity at wavelength #206
217	spectrometer intensity at wavelength #207
218	spectrometer intensity at wavelength #208
219	spectrometer intensity at wavelength #209
220	spectrometer intensity at wavelength #210
221	spectrometer intensity at wavelength #211
222	spectrometer intensity at wavelength #212
223	spectrometer intensity at wavelength #213
224	spectrometer intensity at wavelength #214
225	spectrometer intensity at wavelength #215
226	spectrometer intensity at wavelength #216
227	spectrometer intensity at wavelength #217
228	spectrometer intensity at wavelength #218
229	spectrometer intensity at wavelength #219
230	spectrometer intensity at wavelength #220
231	spectrometer intensity at wavelength #221
232	spectrometer intensity at wavelength #222
233	spectrometer intensity at wavelength #223

Title: NEON Algorithm Theoretical Basis Document (ATBD): Surface Water Nitrate		Date: 12/04/2018
NEON Doc. #: NEON.DOC.002181	Author: J. Vance	Revision: B

234	spectrometer intensity at wavelength #224
235	spectrometer intensity at wavelength #225
236	spectrometer intensity at wavelength #226
237	spectrometer intensity at wavelength #227
238	spectrometer intensity at wavelength #228
239	spectrometer intensity at wavelength #229
240	spectrometer intensity at wavelength #230
241	spectrometer intensity at wavelength #231
242	spectrometer intensity at wavelength #232
243	spectrometer intensity at wavelength #233
244	spectrometer intensity at wavelength #234
245	spectrometer intensity at wavelength #235
246	spectrometer intensity at wavelength #236
247	spectrometer intensity at wavelength #237
248	spectrometer intensity at wavelength #238
249	spectrometer intensity at wavelength #239
250	spectrometer intensity at wavelength #240
251	spectrometer intensity at wavelength #241
252	spectrometer intensity at wavelength #242
253	spectrometer intensity at wavelength #243
254	spectrometer intensity at wavelength #244
255	spectrometer intensity at wavelength #245
256	spectrometer intensity at wavelength #246
257	spectrometer intensity at wavelength #247
258	spectrometer intensity at wavelength #248
259	spectrometer intensity at wavelength #249
260	spectrometer intensity at wavelength #250
261	spectrometer intensity at wavelength #251
262	spectrometer intensity at wavelength #252
263	spectrometer intensity at wavelength #253
264	spectrometer intensity at wavelength #254
265	spectrometer intensity at wavelength #255
266	spectrometer intensity at wavelength #256
267	Temperature of sensor
268	Spectrometer temperature
269	Lamp temperature
270	Cumulative lamp time
271	Relative humidity

Title: NEON Algorithm Theoretical Basis Document (ATBD): Surface Water Nitrate		Date: 12/04/2018
NEON Doc. #: NEON.DOC.002181	Author: J. Vance	Revision: B

272	Main voltage
273	Lamp voltage
274	Internal voltage
275	Main current
276	Fit aux 1
277	Fit aux 2
278	Fit base 1
279	Fit base 2
280	Fit RMSE
281	CTD Time
282	CTD Salinity
283	CTD Temperature
284	CTD Pressure
285	Check sum of data stream

The nitrate value and other relevant fields for a given measurement are identified in Equations 2 – 5:

$$NO_{3,i} = \{(field)3, <value >\}_i \quad \text{Equation 2}$$

$$H_i = \{(field)271, <value >\}_i \quad \text{Equation 3}$$

$$SpAv_L = \{(field)8, <value >\}_i \quad \text{Equation 4}$$

$$SpAv_D = \{(field)9, <value >\}_i \quad \text{Equation 5}$$

For each burst of measurements, the first measurement is a dark measurement in which the UV lamp is off (dark frame: $\{(field)0 = 0\}$), followed by 20 consecutive light measurements in which the UV lamp is on (light frame: $\{(field)0 = 1\}$). If non-consecutive dark or light frames are encountered, implement the error tracking system since the sensor is not functioning properly. After the dark frame, the first 9 light frames allow for the sensor to stabilize. The 10th through 20th light frames will be averaged to provide the 15-minute L1 nitrate DP according to Equation 6.

$$\overline{NO_3} = \frac{1}{11} \sum_{i=11}^{i=21} NO_{3,i} \quad \text{Equation 6}$$

Where:

$i = 1 \dots 21$ for each measurement in the burst, any measurements beyond the 21st frame (20th light frame) should be ignored.

$NO_{3,i}$ = individual nitrate measurements (light and dark frames)

Title: NEON Algorithm Theoretical Basis Document (ATBD): Surface Water Nitrate		Date: 12/04/2018
NEON Doc. #: NEON.DOC.002181	Author: J. Vance	Revision: B

$\overline{NO_3}$ = average nitrate per burst measurement

If greater than 31 light frames are available for averaging, flag the data with a gap test value of 2, meaning that there were more measurements than expected (this would indicate that neither the old or new SUNA settings are being used). If less than 10 light frames are available for averaging, flag the data with a gap test value of 1, meaning that there were fewer measurements than expected. Similarly, if greater than 1 dark frame are present, flag the data with gap test value of 3, meaning that there were more measurements than expected. If less than 1 dark frames are present, flag the data with gap test value of 4, meaning that there were less measurements than expected.

The time between the initiation of bursts ($i = 1$) should be 00:15:00. Each burst should last a maximum of $21 \times 1.5s = 00:00:31.5$ (NOTE: while the configuration changes are implemented, sensor that are not yet updated will have a burst of $51 \times 1.5s = 00:01:16.5$). Therefore, the total time step between the end of a burst and the beginning of the next burst should be $t \geq 00:12:00$.

Each L1 15-minute nitrate measurement value shall have a startDate timestamp of the first measurement included in the mean and an endDate timestamp of the last measurement included in the mean.

The timestamp of individual measurements may be used to find the beginning of each burst. The measurement index is then reset to 1 at the beginning of each burst as follows:

While $i \leq n$

$$i = \begin{cases} 1 & \text{if } t_{i+1} - t_i > 00:10:00.0 \\ i + 1 & \text{otherwise} \end{cases}$$

5 ALGORITHM IMPLEMENTATION

Data flow for signal processing of L1 DPs will be treated in the following order.

1. Extract L0 values from the appropriate fields of the concatenated data stream for each instantaneous light or dark frame according to Eq. 1.
2. Find the beginning of the burst measurement according to Section 4.
3. QA/QC sensor flags will be applied to the data stream values within the averaging window defined in Eq. 6, details below.

Title: NEON Algorithm Theoretical Basis Document (ATBD): Surface Water Nitrate		Date: 12/04/2018
NEON Doc. #: NEON.DOC.002181	Author: J. Vance	Revision: B

4. QA/QC Plausibility tests will be applied to the nitrate measurements (field 3 only) within the averaging window defined in Eq. 6 in accordance with AD[06], details are provided below.
5. Signal de-spiking will be applied to the nitrate measurements (field 3 only) within the averaging window defined in Eq. 6 in accordance with AD[07].
6. Nitrate measurement averages will be calculated using Eq. 6.
7. Descriptive statistics, i.e. minimum, maximum, and variance, will be determined for each burst measurement of surface water nitrate.
8. Quality metrics, quality flags, and the final quality flag will be produced for each nitrate measurement according to AD[12].

QA/QC Procedure:

1. **Plausibility Tests** AD[06] – All plausibility tests will be determined for the nitrate analyzer. Test parameters will be provided by AIS and maintained in the CI data store. All plausibility tests will be applied to the sensor’s converted LO DPs and associated quality flags (QFs) will be generated for each test.
2. **Sensor Flags** – Recently it was found that the internal humidity of this sensor can reach levels that impair the both the health and operation of the sensor. Therefore, we will check the humidity level for each measurement and measurements taken when the humidity is above the threshold of 40% will be flagged accordingly.

Additionally, the spectral average measured during light frames should far exceed the value of the spectral average measured during dark frames. The dark frames are taken with the lamp off and provide the background signal of the detector. If the spectral average of the light frame is not greater than at least twice that of the dark frames that measurement shall be flagged accordingly. The dark and spectral averages are calculated internally by the SUNA and no averaging is done by CI for this. Only the output values for a given measurement are compared for data quality assurance.

a. Spectral Average:

$$\text{SpecQF} = \begin{cases} 1 & \text{if } SpAv_L \leq 2 \times SpAv_D \\ 0 & \text{otherwise} \end{cases}$$

b. Internal Humidity:

$$\begin{cases} 1 & \text{if } H_i \geq 40 \end{cases}$$

Title: NEON Algorithm Theoretical Basis Document (ATBD): Surface Water Nitrate		Date: 12/04/2018
NEON Doc. #: NEON.DOC.002181	Author: J. Vance	Revision: B

$$\text{humidityQF} = \begin{cases} \text{[unspecified]} \\ 0 \text{ otherwise} \end{cases}$$

3. **Signal Despiking** Time segments and threshold values for the automated despiking QA/QC routine will be specified by AIS and maintained in the CI data store. QFs from the despiking analysis will be applied according to AD[07].
4. **Quality Flags (QFs) and Quality Metrics (QMs)** AD[12] – If a datum fails one of the following tests it will not be used to create a L1 DP, *sensor test, despiking, range, persistence, and step*. α and β QFs and QMs will be determined for nitrate using the flags in Table 3. In addition, nitrate L1 DPs will have a QA/QC report and quality metrics associated with each flag listed in Table 4, as detailed in AD[12]. Ancillary information needed for the algorithm and other information maintained in the CI data store is shown in Table 4. The final quality flag for surface water nitrate will be determined accordingly.

Table 5-1: Flags associated with Surface Water Nitrate measurements.

Tests
Null
Gap
Range
Persistence
Signal Despiking
Step
Sensor Test – Internal Humidity
Sensor Test – Spectral Average
Alpha
Beta

Title: NEON Algorithm Theoretical Basis Document (ATBD): Surface Water Nitrate		Date: 12/04/2018
NEON Doc. #: NEON.DOC.002181	Author: J. Vance	Revision: B

Tests
Final Quality Flag

Table 5-2: Information maintained in the CI data store for Surface Water Nitrate.

Tests/Values	CI Data Store Contents
Null	Test limit
Gap	Test limit
Range	Minimum and maximum values
Persistence	Window size, threshold values and maximum time length
Step	Threshold values
Signal Despiking	Time segments and threshold values
Sensor Test – Internal Humidity	Humidity threshold of 40 %
Sensor Test – Spectral Average	Light / Dark Spectral Average Ratio minimum of 2
Uncertainty	AD[09]
Final Quality Flag	AD[12]

6 UNCERTAINTY

Uncertainty of measurement is inevitable (JCGM 2008, 2012; Taylor 1997). It is crucial that uncertainties are identified and quantified to determine statistical interpretations about mean quantity and variance structure; both are important when constructing higher level data products (e.g. L1 DP) and modeled processes. Uncertainty related to the Surface Water Nitrate and associated data products is provided in detail in the Aquatics Uncertainty Document AD [09], which serves to identify, evaluate, and quantify sources of uncertainty relating to L1 surface water nitrate and L1 surface water nitrate DPs. It is a reflection of the information described in AD[08] and is explicitly described for the nitrate sensor in AD [09].

6.1 Uncertainty of Surface Water Nitrate

Uncertainty of the SUNA nitrate analyzer assembly is discussed in this section. The section is broken down into two topics. The first informs the sources of *measurement* uncertainty, i.e., those associated with *individual nitrate measurements*. The second details uncertainties associated with temporally averaged data products. A diagram detailing the data flow and known sources of uncertainty are displayed in Figure 04.

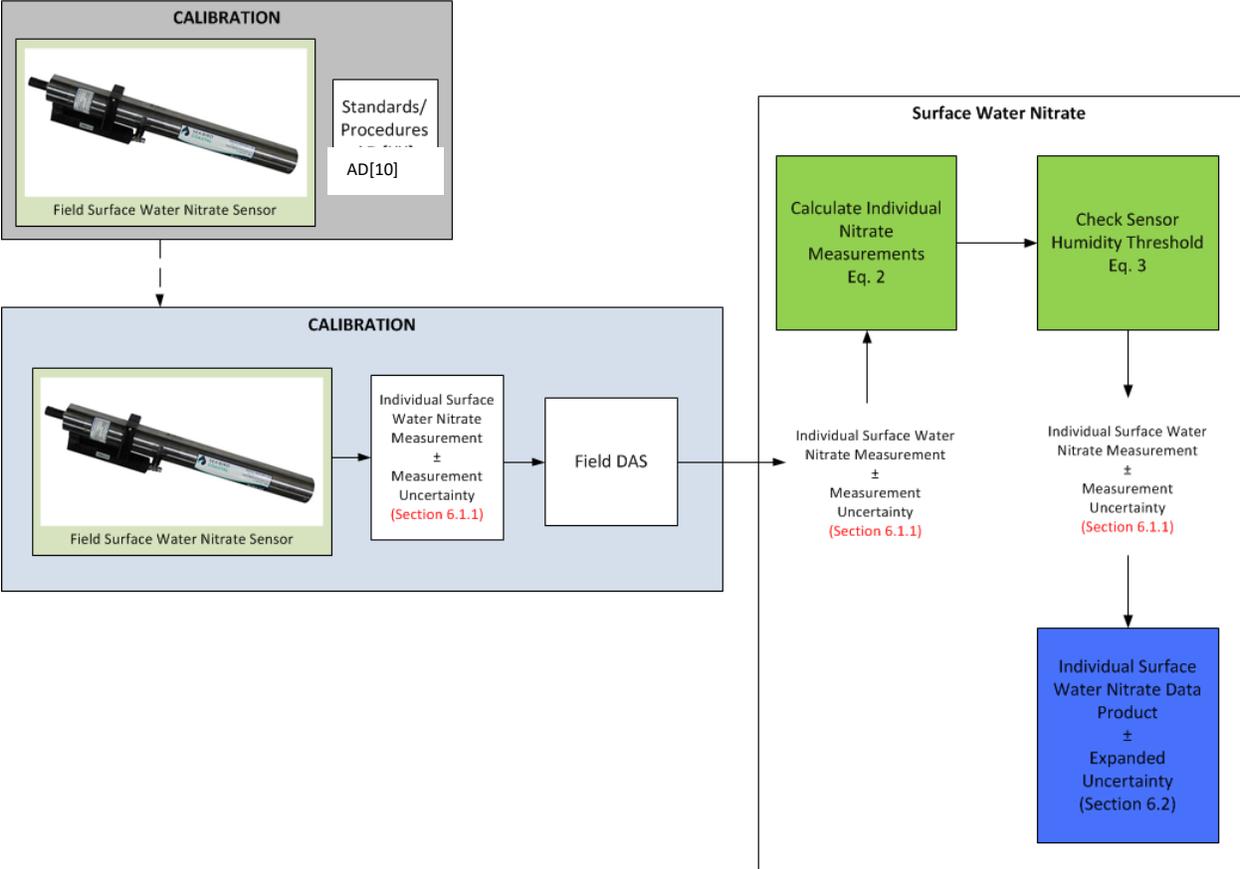


Figure 3. Displays the data flow and associated uncertainties of individual measurements of surface water nitrate and associated L1 DPs.

6.1.1 Measurement Uncertainty

The following subsections present the uncertainties associated with *individual observations*. It is important to note that the uncertainties presented in the following subsections are *measurement uncertainties*, that is, they reflect the uncertainty of an *individual* measurement. These uncertainties should not be confused with those presented in Section 6.1.2. We urge the reader to refer to AD[11] for further details concerning the discrepancies between quantification of measurement uncertainties and L1 uncertainties.

Title: NEON Algorithm Theoretical Basis Document (ATBD): Surface Water Nitrate		Date: 12/04/2018
NEON Doc. #: NEON.DOC.002181	Author: J. Vance	Revision: B

NEON calculates measurement uncertainties according to recommendations of the Joint Committee for Guides in Metrology (JCGM) 2008. In essence, if a measurand y is a function of n input quantities

x_i ($i = 1, \dots, n$), *i.e.*, $y = f(x_1, x_2, \dots, x_n)$, the combined measurement uncertainty of y , assuming the inputs are independent, can be calculated as follows:

$$u_c(y) = \left(\sum_{i=1}^n \left(\frac{\partial f}{\partial x_i} \right)^2 u^2(x_i) \right)^{\frac{1}{2}} \quad \text{Equation 7}$$

where

$\frac{\partial f}{\partial x_i}$ =partial derivative of y with respect to x_i

$u(x_i)$ =combined standard uncertainty of x_i .

Thus, the uncertainty of the measurand can be found by summing the input uncertainties in quadrature. For surface water nitrate measurements, the sources of uncertainty are discussed below.

6.1.1.1 DAS

The SUNA V2 nitrate sensor has an internal Analog to Digital (A/D) converter and outputs data in digital form. Therefore, no data conversions occur within the DAS, and uncertainty introduced by the DAS can be considered negligible.

6.1.1.2 Calibration

The SUNA V2 is calibrated by the manufacturer Satlantic LP and no additional calibration is currently performed by CVAL. The accuracy of calibrated measurements are given by the manufacturer. Additionally the sensor baseline (blank) is calibration in the field. If the sensor is properly field-calibrated, the nitrate concentration should have an accuracy as follows:

$$\text{Measurement Accuracy} = \begin{cases} 2 \mu M & \text{if } \overline{NO_3} \leq 20 \mu M \\ \overline{NO_3} \times 10\% & \text{if } 20 \mu M < NO_{3,i} \leq 1000 \mu M \end{cases}$$

The values 0-1000 μM represent the expected environmental range across the NEON Aquatic Sites. The uncertainty is assumed to be the manufacturer's reported accuracy divided by 3. Therefore, the uncertainty will be 0.666 μM (u_{A1}) or 3.33% (u_{A3}) of the measurement, depending on the concentration of the individual measurements. These values will be given by CVAL as $\{u_{A1}\}$ and $\{u_{A3}\}$

Title: NEON Algorithm Theoretical Basis Document (ATBD): Surface Water Nitrate		Date: 12/04/2018
NEON Doc. #: NEON.DOC.002181	Author: J. Vance	Revision: B

(see Section 2.4) representing i) the repeatability and reproducibility of the sensor and ii) uncertainty of the calibration procedures and coefficients including uncertainty in the standard (truth). This will be provided by CVAL, stored in the CI data store, and applied to all *individual nitrate measurements*. CI will need to use the appropriate uncertainty value for individual measurements based on the concentration as follows:

$$\text{Individual measurement uncertainty } \{u_{An}\} = \begin{cases} u_{A1} & \text{if } \overline{NO_3} \leq 20 \mu M \\ u_{A3}, & \text{if } 20 \mu M < \overline{NO_3} \leq 1000 \mu M \end{cases}$$

6.1.1.3 Combined Measurement Uncertainty

Because the only known quantifiable uncertainties are those provided by the manufacturer, the combined uncertainty of nitrate is simply a product to the standard uncertainty value given by the manufacturer and provided by CVAL, u_{A1} , (See Sections 2.4 and 6.1.1.2).

$$u_{CAL}(\overline{NO_3}) = \begin{cases} u_{An} & \text{if } \overline{NO_3} \leq 20 \mu M \\ u_{An} \times \overline{NO_3} & \text{if } 20 \mu M < \overline{NO_3} \leq 1000 \mu M \end{cases} \quad \text{Equation 8}$$

Where,

- $u_{CAL}(\overline{NO_3})$ = standard calibration uncertainty of an individual measurement (μM)
- u_{An} = u_{A1} or u_{A3} , depending on concentration range as identified in 6.1.1.2, calibration uncertainty provided by CVAL (% from manufacturer)
- $\overline{NO_3}$ = averaged nitrate measurements (μM)

6.1.2 Uncertainty of the L1 Mean Data Products

The following subsections discuss uncertainties associated with temporally averaged, i.e., L1 mean data products. As stated previously, it is important to note the differences between the *measurement*

Title: NEON Algorithm Theoretical Basis Document (ATBD): Surface Water Nitrate		Date: 12/04/2018
NEON Doc. #: NEON.DOC.002181	Author: J. Vance	Revision: B

uncertainties presented in Section 6.1.1 and the uncertainties presented in the following subsections. The uncertainties presented in the following subsections reflect the uncertainty of a time-averaged mean value, that is, they reflect the uncertainty of a distribution of measurements collected under non-controlled conditions (i.e., those found in the field), as well as any uncertainties in the form of *Truth* and *Trueness* related to the accuracy of the field assembly.

6.1.2.1 Repeatability (Natural Variation)

To quantify the uncertainty attributable to random effects, the distribution of the individual measurements is used. Specifically, the *estimated standard error of the mean (natural variation)* is computed. This value reflects the repeatability of measurements for a specified time period:

$$u_{NAT}(\overline{NO_3}) = \sqrt{\frac{\sigma^2}{n}} \quad \text{Equation 9}$$

Where

$\overline{NO_3}$ = averaged nitrate measurements (μM)

$u_{NAT}(\overline{NO_3})$ = standard error of the mean (natural variation)

σ = standard deviation of individual within the averaging window (of the burst)

n = number of observations made within the averaging window (of the burst)

6.1.2.2 Calibration

The calibration uncertainty for a L1 mean DP is similar to that described in Section 6.1.1.1. However, the uncertainties provided by CVAL (see Section 2.4) do not account for i) individual sensor repeatability, or ii) the variation of sensors' responses over a population (reproducibility). These components estimate the uncertainties due to the accuracy of the instrumentation in the form of *Truth* and *Trueness*, a quantity that is not captured by the standard error of the mean. This is a constant value that will be provided by CVAL and stored in the CI data store. Please refer to AD[10] for further justification regarding evaluation and quantification of this combined uncertainty.

6.1.2.3 Combined Uncertainty

The combined uncertainty for L1 data products are computed by summing the uncertainties from Section 6.1.2.1 and the CVAL provided uncertainties in quatrature:

$$u_c(\overline{NO_3}) = [u_{NAT}^2(\overline{NO_3}) + u_{CAL}^2(\overline{NO_3})]^{1/2} \quad \text{Equation 10}$$

6.1.2.4 Communicating Precision

L1 mean surface water nitrate data products will be reported to 0.1 μM . The sensor is capable of measuring nitrate at a precision of 0.3 μM . The resolution of individual nitrate measurements is 0.1 μM ,

Title: NEON Algorithm Theoretical Basis Document (ATBD): Surface Water Nitrate		Date: 12/04/2018
NEON Doc. #: NEON.DOC.002181	Author: J. Vance	Revision: B

as this maintains the proper significant figures, despite the reported resolution being greater than the 0.3 μM precision and limit of detection.

6.2 Expanded Uncertainty

We assume the measurement variability is normally distributed (Gaussian). The combined uncertainty represents plus or minus one standard deviation or a confidence interval of 68%. This confidence level is below the industry standard and is therefore expanded to a 95% confidence interval. This is typically calculated by multiplying the combined uncertainty, $u_{c,r}(y)$, by a coverage factor, k_p .

$$U_p = k_p u_{c,r}(y) \quad \text{Equation 11}$$

Where $k_{95} = 1.96$ for $p = 95$ for a given degrees of freedom. k_p is approximated by a t-distribution with an effective degrees of freedom, v_{eff} , obtained from the Welch-Satterwaite formula:

$$v_{eff} = \frac{u_c^4(y)}{\sum_{i=1}^n \frac{u_i^4(y)}{v_i}} \quad \text{Equation 12}$$

The coverage factor then becomes $k_p = t_p(v_{eff})$, where $t_p(v_{eff})$ is obtained from a table.

However to simplify the calculations further, we can conservatively estimate the expanded uncertainty at a 95% confidence level to be two times the combined uncertainty.

$$U_{Expanded} = 2 \times u_c \quad \text{Equation 13}$$

This expansion is to be applied to all combined uncertainties for the L1 DP described herein.

6.1 Uncertainty Budget

The uncertainty budget is a visual aid detailing i) quantifiable sources of uncertainty, ii) means by which they are derived, and iii) the order of their propagation. Uncertainty values denoted in this budget are either derived within this document or are provided by other NEON teams (e.g., CVAL), and stored in the CI data store.

Table 3. Uncertainty budget for individual measurements. Shaded rows denote the order of uncertainty propagation (from lightest to darkest).

Source of Measurement Uncertainty	Measurement uncertainty Component $u(x_i)$	Measurement Uncertainty Value	$\frac{\partial f}{\partial x_i}$	$u_{x_i}(Y) \equiv \left \frac{\partial f}{\partial x_i} \right u(x_i)$
Nitrate	$u_{CAL}(NO_{3,i})$	AD[11]	n/a	Eq. 9

Table 4. Uncertainty budget for L1 mean DPs. Shaded rows denote the order of uncertainty propagation (from lightest to darkest).

Source of Uncertainty	Uncertainty Component $u(x)$	Uncertainty Value	$\frac{\partial f}{\partial x_i}$	$u_{u_{x_i}}(Y) \equiv \left \frac{\partial f}{\partial x_i} \right u(x_i)$
Nitrate	$u_c(\overline{NO_3})$	Eq. (11)	n/a	Eq. 11
Calibration	$u_{CAL}(NO_{3,i})$	AD[11]	n/a	Eq. 9
Natural variation	$u_{NAT}(\overline{NO_3})$	Eq. 10	n/a	Eq. 10

7 FUTURE PLANS AND MODIFICATIONS

Future system flags may be incorporated into the data stream and included in the QA/QC summary DP ($Qsum_{5min}$) that summarizes any flagged data that went into the computation of the L1 DP.

It is planned to add another sensor flag that will identify when the internal temperature of the sensor has exceeded 35°C. At this temperature, the sensor shuts off. Providing this additional sensor flag will provide clarity when expected data is missing and no other flags are thrown.

Future implementation of an additional data filter pass for quality control over longer temporal scales is planned.

It is planned that CVAL will provide an internal, independent calibration for performance of the SUNA in freshwater and at low concentrations. Once implemented CVAL will perform a three-point calibration with the associated coefficients.

8 BIBLIOGRAPHY

Satlantic LP (2014) Satlantic SUNA Manual for SUNA running firmware version 2.5 or later, SAT-DN-00628, Rev. E., <http://satlantic.com/sites/default/files/documents/Satlantic-SUNA-V2-Manual-Rev-E.pdf>

JCGM (2012) International vocabulary of metrology – Basic and general concepts and associated terms (VIM). 3rd Edition. pp. 92

Taylor, J. R. (1997) An Introduction to Error Analysis: The Study of Uncertainties in Physical Measurements. University Science Books, Mill Valley, California. 2nd Ed. pp. 327.